

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080924AL\
 Data File : FE049544.D
 Signal(s) : FID1B.ch
 Acq On : 09 Aug 2024 20:06
 Operator : YP\AJ
 Sample : P3479-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 10 01:22:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 071724.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 17 14:26:40 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.327	5894629	50.452 ug/ml
Spiked Amount 50.000		Recovery =	100.90%
Target Compounds			
4) T n-Dodecane (C12)	6.696	82811	0.538 ug/ml
6) T n-Tetradecane (C14)	8.523	87391	0.576 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080924AL\
Data File : FE049544.D
Signal(s) : FID1B.ch
Acq On : 09 Aug 2024 20:06
Operator : YP\AJ
Sample : P3479-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 10 01:22:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 071724.M
Quant Title : GC Extractables
QLast Update : Wed Jul 17 14:26:40 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

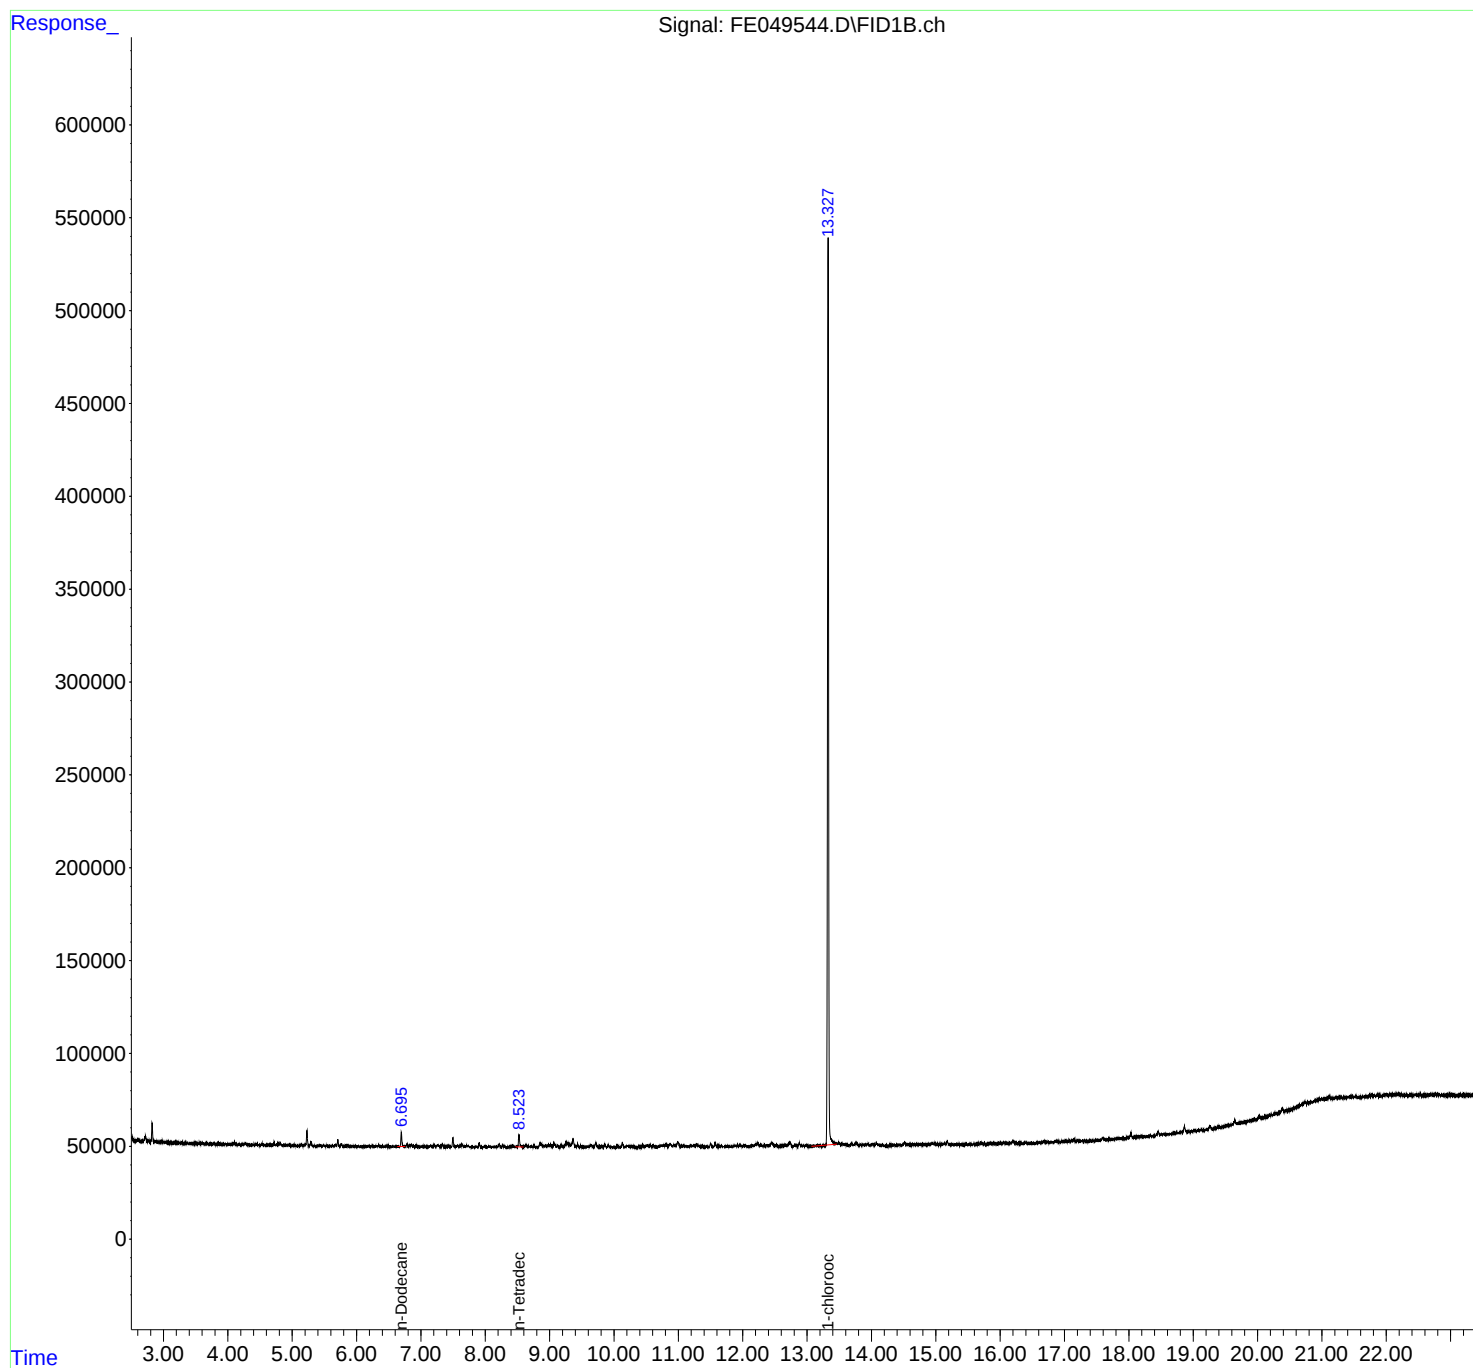


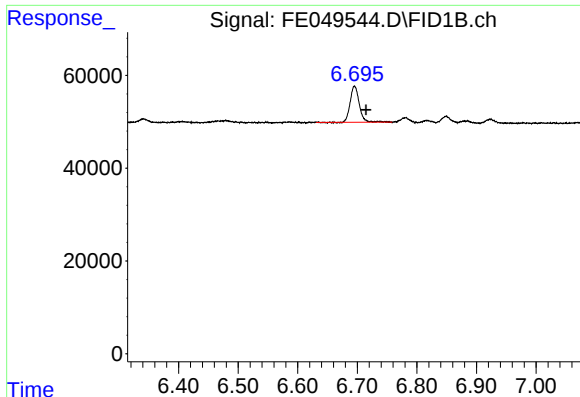

#4 n-Dodecane (C12)


R.T.: 6.696 min
Delta R.T.: -0.020 min
Response: 82811
Conc: 0.54 ug/ml

Instrument :
FID_E
ClientSampleId :

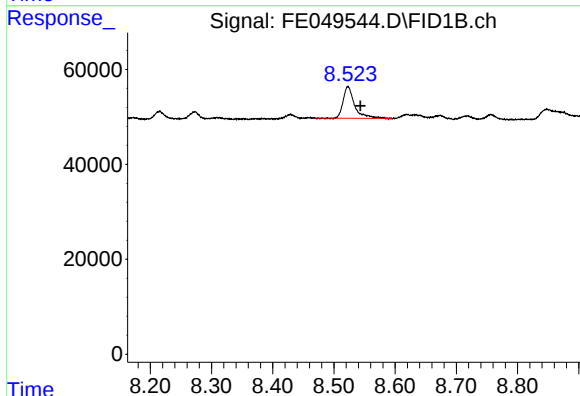


#6 n-Tetradecane (C14)

R.T.: 8.523 min
Delta R.T.: -0.020 min
Response: 87391
Conc: 0.58 ug/ml

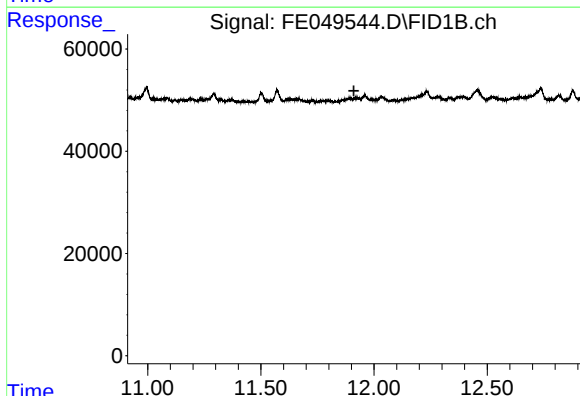

#9 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 11.911 min
Response: 0
Conc: N.D.

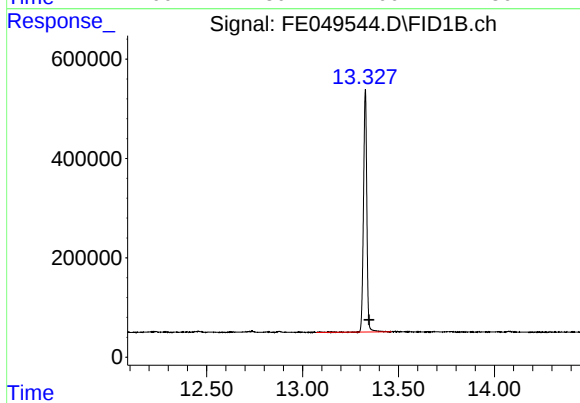

#12 1-chlorooctadecane (SURRE)

R.T.: 13.327 min
Delta R.T.: -0.020 min
Response: 5894629
Conc: 50.45 ug/ml