

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE081318\
 Data File : FE028552.D
 Signal(s) : FID1B.CH
 Acq On : 13 Aug 2018 18:48
 Operator : AJ\SJ
 Sample : J4447-12MS
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 14 07:09:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE071918.M
 Quant Title :
 QLast Update : Fri Jul 20 01:13:49 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.974	2617407	15.363 ug/ml
Target Compounds			
1) N-OCTANE	2.560	1451750	16.338 ug/ml
6) N-TETRADECANE	8.561	695618	6.005 ug/ml
8) N-OCTADECANE	11.552	2884953	21.808 ug/ml
9) N-EICOSANE	12.956	165614	1.216 ug/ml
10) N-TETRACOSANE	15.180	3072671	23.005 ug/ml
11) N-OCTACOSANE	17.159	2854447	23.430 ug/ml
12) N-DOTRIACONTANE	18.886	2763968	24.170 ug/ml
14) N-HEXATRIACONTANE	20.412	994951	9.047 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE081318\
Data File : FE028552.D
Signal(s) : FID1B.CH
Acq On : 13 Aug 2018 18:48
Operator : AJ\SJ
Sample : J4447-12MS
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 14 07:09:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE071918.M
Quant Title :
QLast Update : Fri Jul 20 01:13:49 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

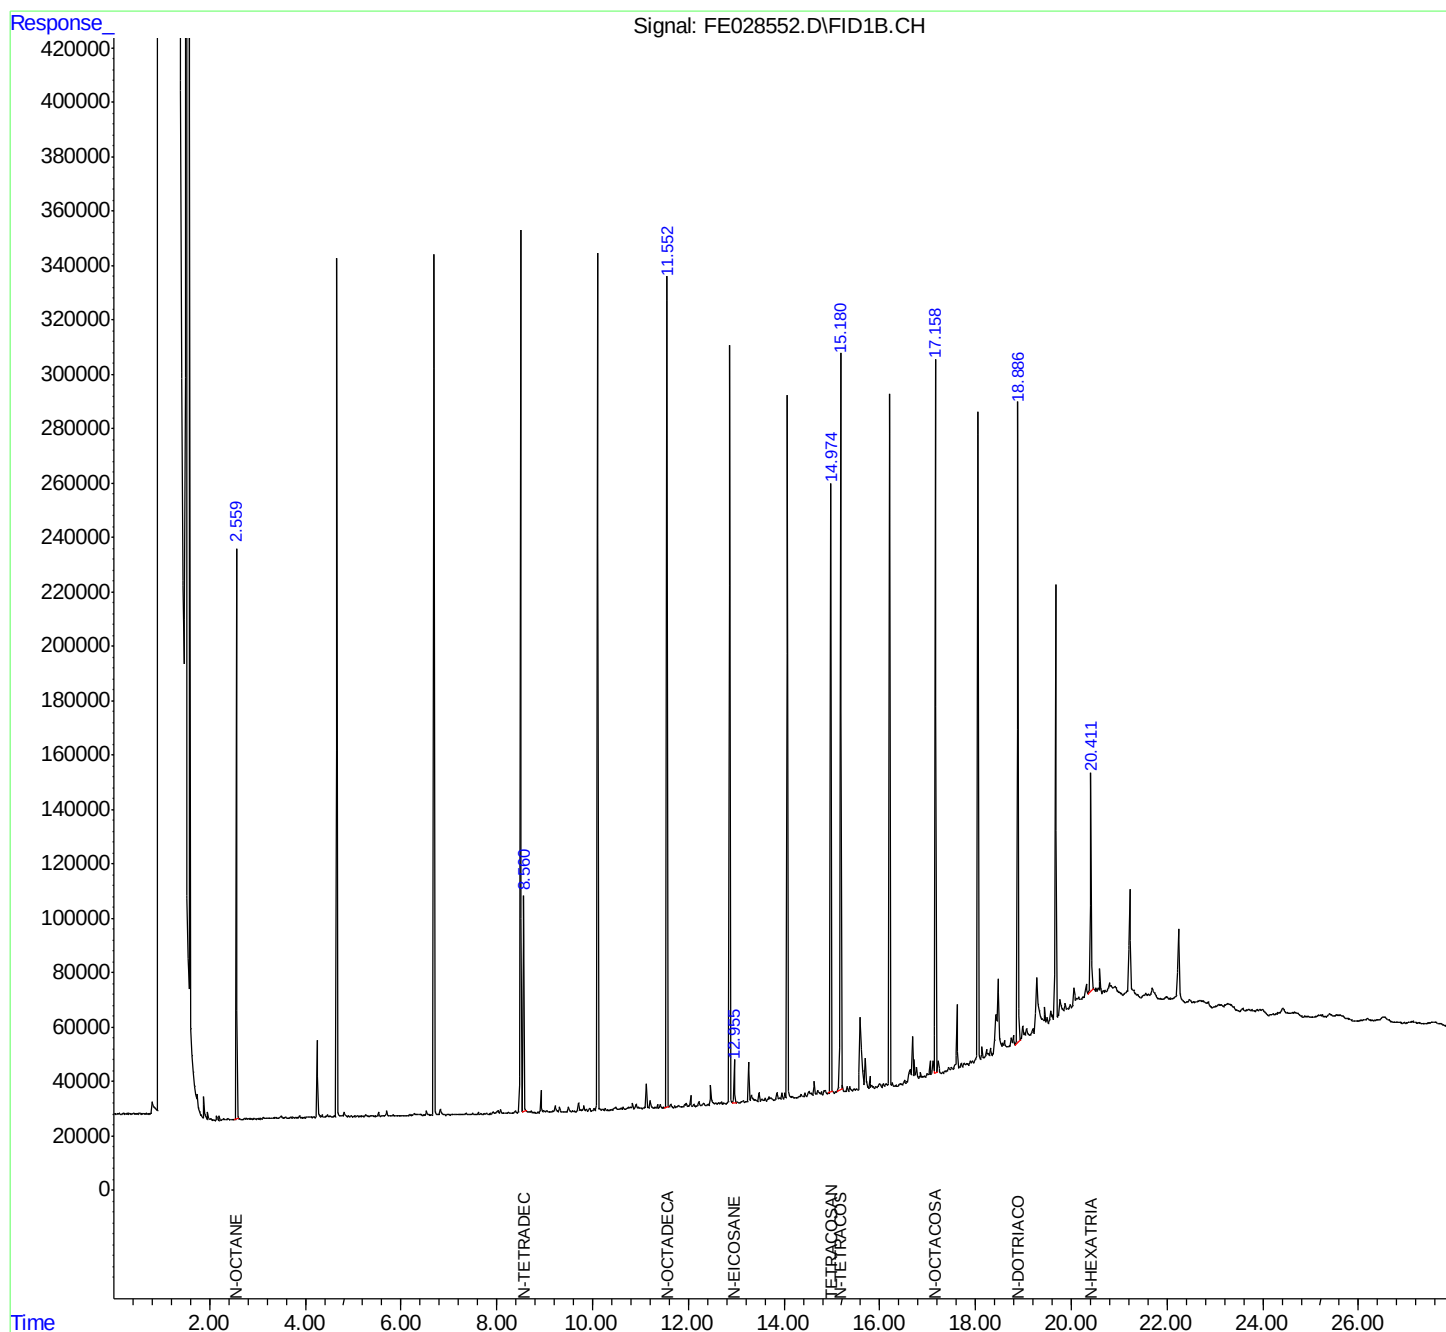

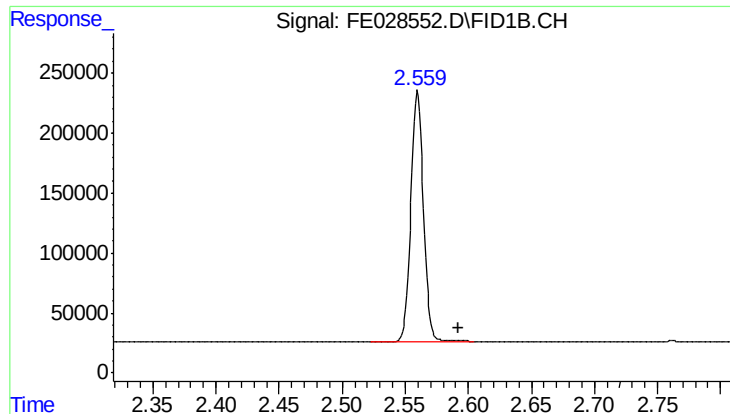


#1 N-OCTANE

R.T.: 2.560 min
Delta R.T.: -0.032 min
Response: 1451750
Conc: 16.34 ug/ml

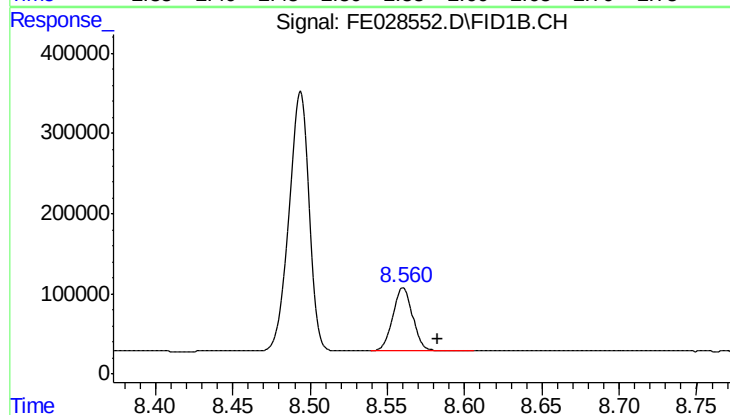


#6 N-TETRADECANE

R.T.: 8.561 min
Delta R.T.: -0.022 min
Response: 695618
Conc: 6.00 ug/ml

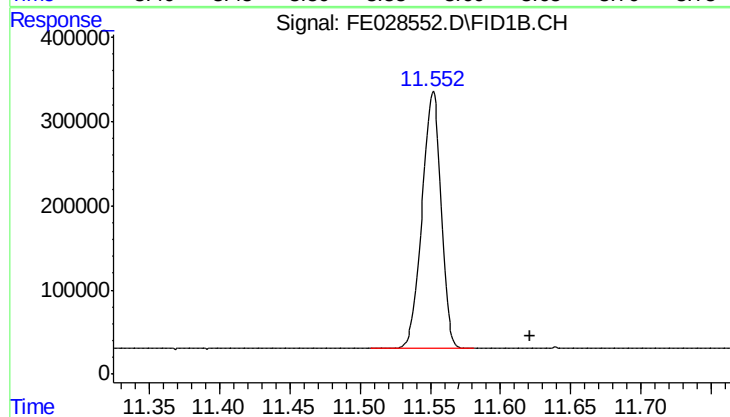


#8 N-OCTADECANE

R.T.: 11.552 min
Delta R.T.: -0.069 min
Response: 2884953
Conc: 21.81 ug/ml

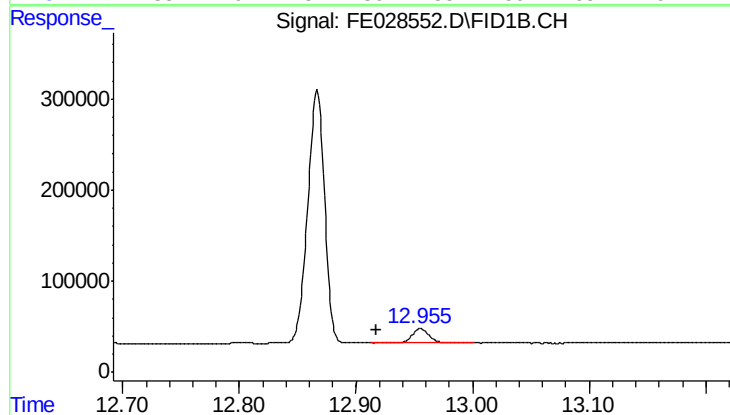


#9 N-EICOSANE

R.T.: 12.956 min
Delta R.T.: 0.038 min
Response: 165614
Conc: 1.22 ug/ml

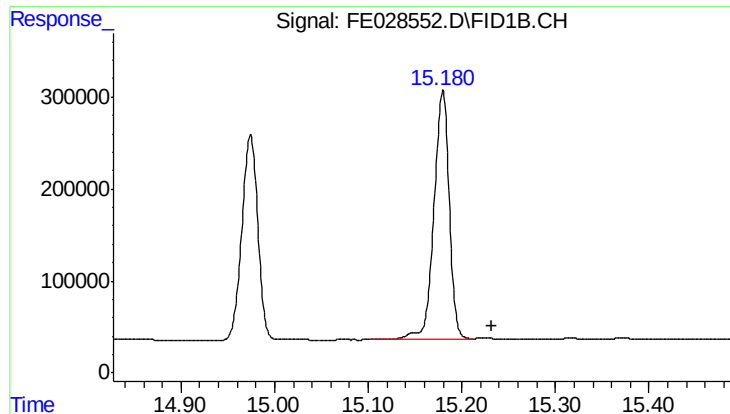


#10 N-TETRACOSANE

R.T.: 15.180 min
Delta R.T.: -0.052 min
Response: 3072671
Conc: 23.00 ug/ml

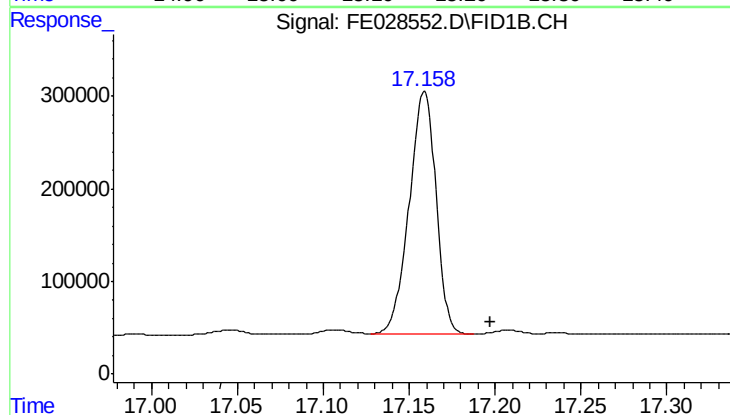


#11 N-OCTACOSANE

R.T.: 17.159 min
Delta R.T.: -0.038 min
Response: 2854447
Conc: 23.43 ug/ml

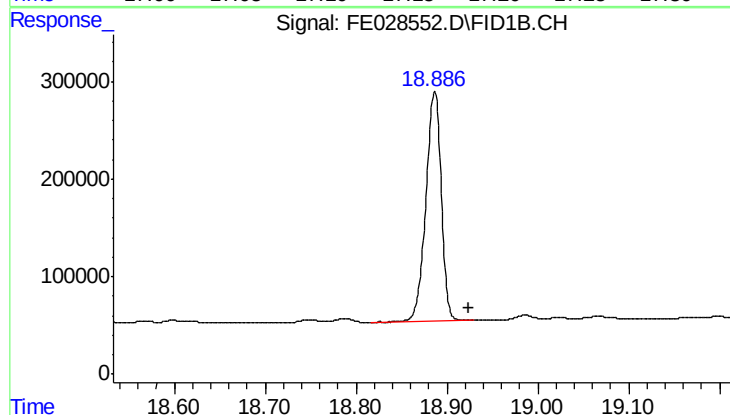


#12 N-DOTRIACONTANE

R.T.: 18.886 min
Delta R.T.: -0.038 min
Response: 2763968
Conc: 24.17 ug/ml

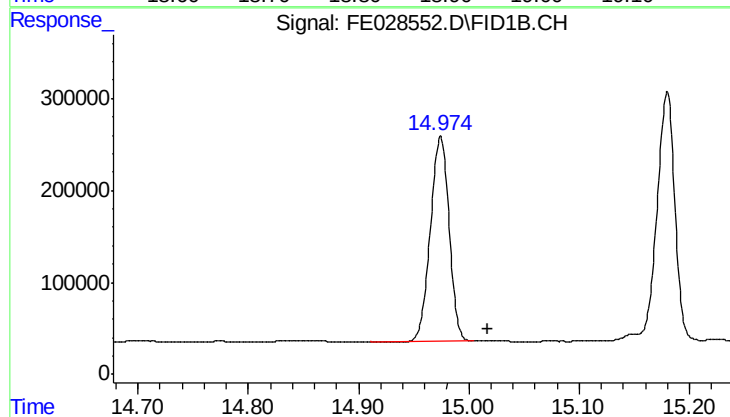

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.974 min
Delta R.T.: -0.042 min
Response: 2617407
Conc: 15.36 ug/ml

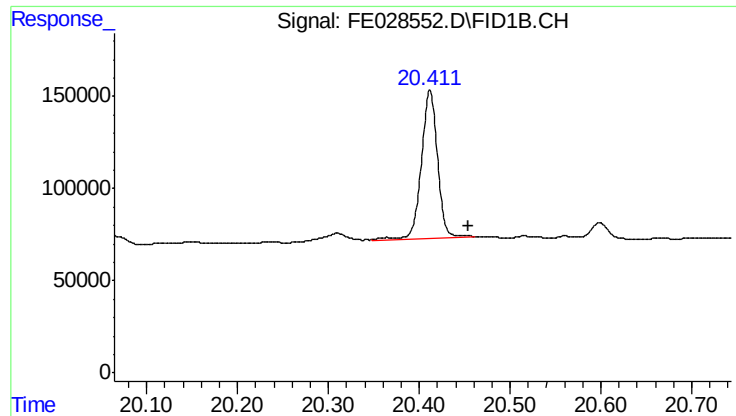

#14 N-HEXATRIACONTANE

R.T.: 20.412 min
Delta R.T.: -0.042 min
Response: 994951
Conc: 9.05 ug/ml