

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE081425AL\  
 Data File : FE055305.D  
 Signal(s) : FID1B.ch  
 Acq On : 14 Aug 2025 18:00  
 Operator : YP\AJ  
 Sample : Q2844-04  
 Misc :  
 ALS Vial : 16 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 MOO-25-0234-0235

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 08/15/2025  
 Supervised By :mohammad ahmed 08/18/2025

Integration File: autoint1.e  
 Quant Time: Aug 14 18:28:12 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 080125.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Aug 01 13:47:09 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units    |
|--------------------------------|--------|------------|---------------|
| -----                          |        |            |               |
| System Monitoring Compounds    |        |            |               |
| 9) S ortho-Terphenyl (SURR)    | 12.090 | 6012663    | 42.104 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 84.21%        |
| 12) S 1-chlorooctadecane (S... | 13.519 | 618367     | 5.751 ug/mlm  |
| Spiked Amount 50.000           |        | Recovery = | 11.50%        |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE081425AL\  
Data File : FE055305.D  
Signal(s) : FID1B.ch  
Acq On : 14 Aug 2025 18:00  
Operator : YP\AJ  
Sample : Q2844-04  
Misc :  
ALS Vial : 16 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
MOO-25-0234-0235


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 08/15/2025  
Supervised By :mohammad ahmed 08/18/2025

Integration File: autoint1.e  
Quant Time: Aug 14 18:28:12 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 080125.M  
Quant Title : GC Extractables  
QLast Update : Fri Aug 01 13:47:09 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

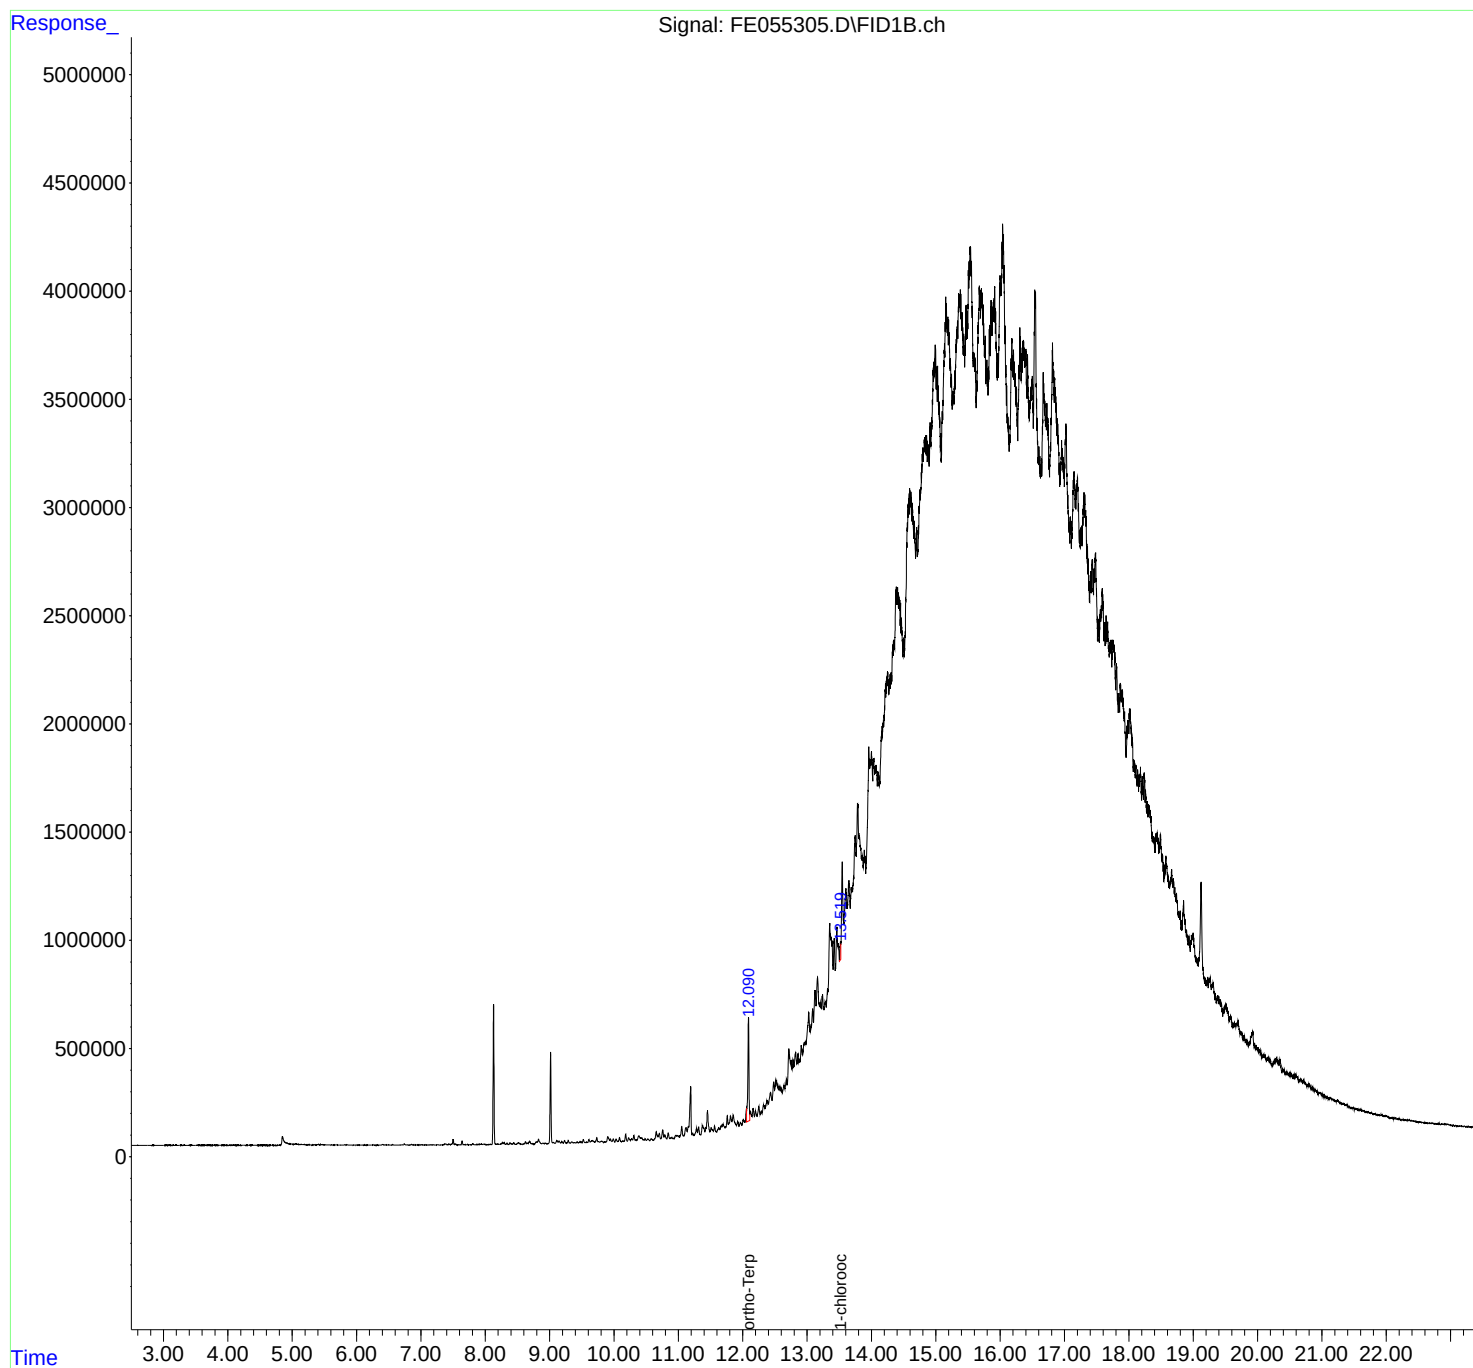

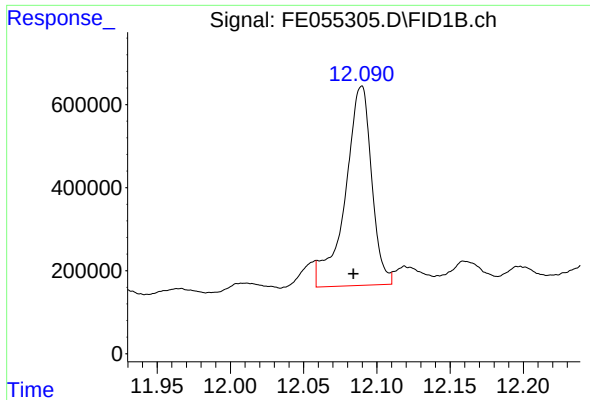


#9 ortho-Terphenyl (SURR)

R.T.: 12.090 min  
Delta R.T.: 0.006 min  
Response: 6012663  
Conc: 42.10 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
MOO-25-0234-0235

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 08/15/2025  
Supervised By :mohammad ahmed 08/18/2025

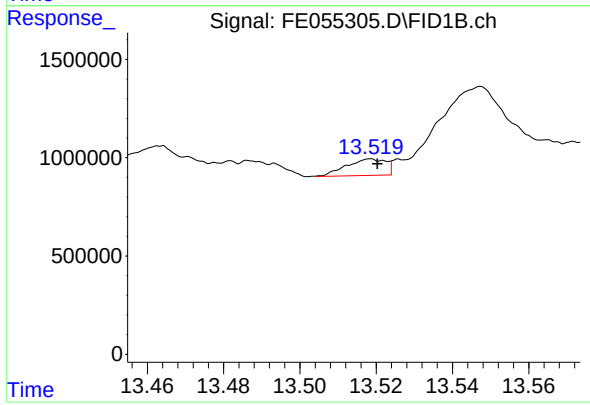

#12 1-chlorooctadecane (SURR)

R.T.: 13.519 min  
Delta R.T.: -0.002 min  
Response: 618367  
Conc: 5.75 ug/ml m