

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE081523AL\
 Data File : FE043976.D
 Signal(s) : FID1B.ch
 Acq On : 16 Aug 2023 01:21
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 16 02:24:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 080323.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 02 09:56:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
19) T n-Tetratriacontane (C34)	19.724	129861	0.874 ug/ml
21) T n-Octatriacontane (C38)	21.266f	235494	1.765 ug/ml
22) T n-Tetracontane (C40)	22.099	786363	6.095 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE081523AL\
Data File : FE043976.D
Signal(s) : FID1B.ch
Acq On : 16 Aug 2023 01:21
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 16 02:24:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 080323.M
Quant Title : GC Extractables
QLast Update : Wed Aug 02 09:56:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

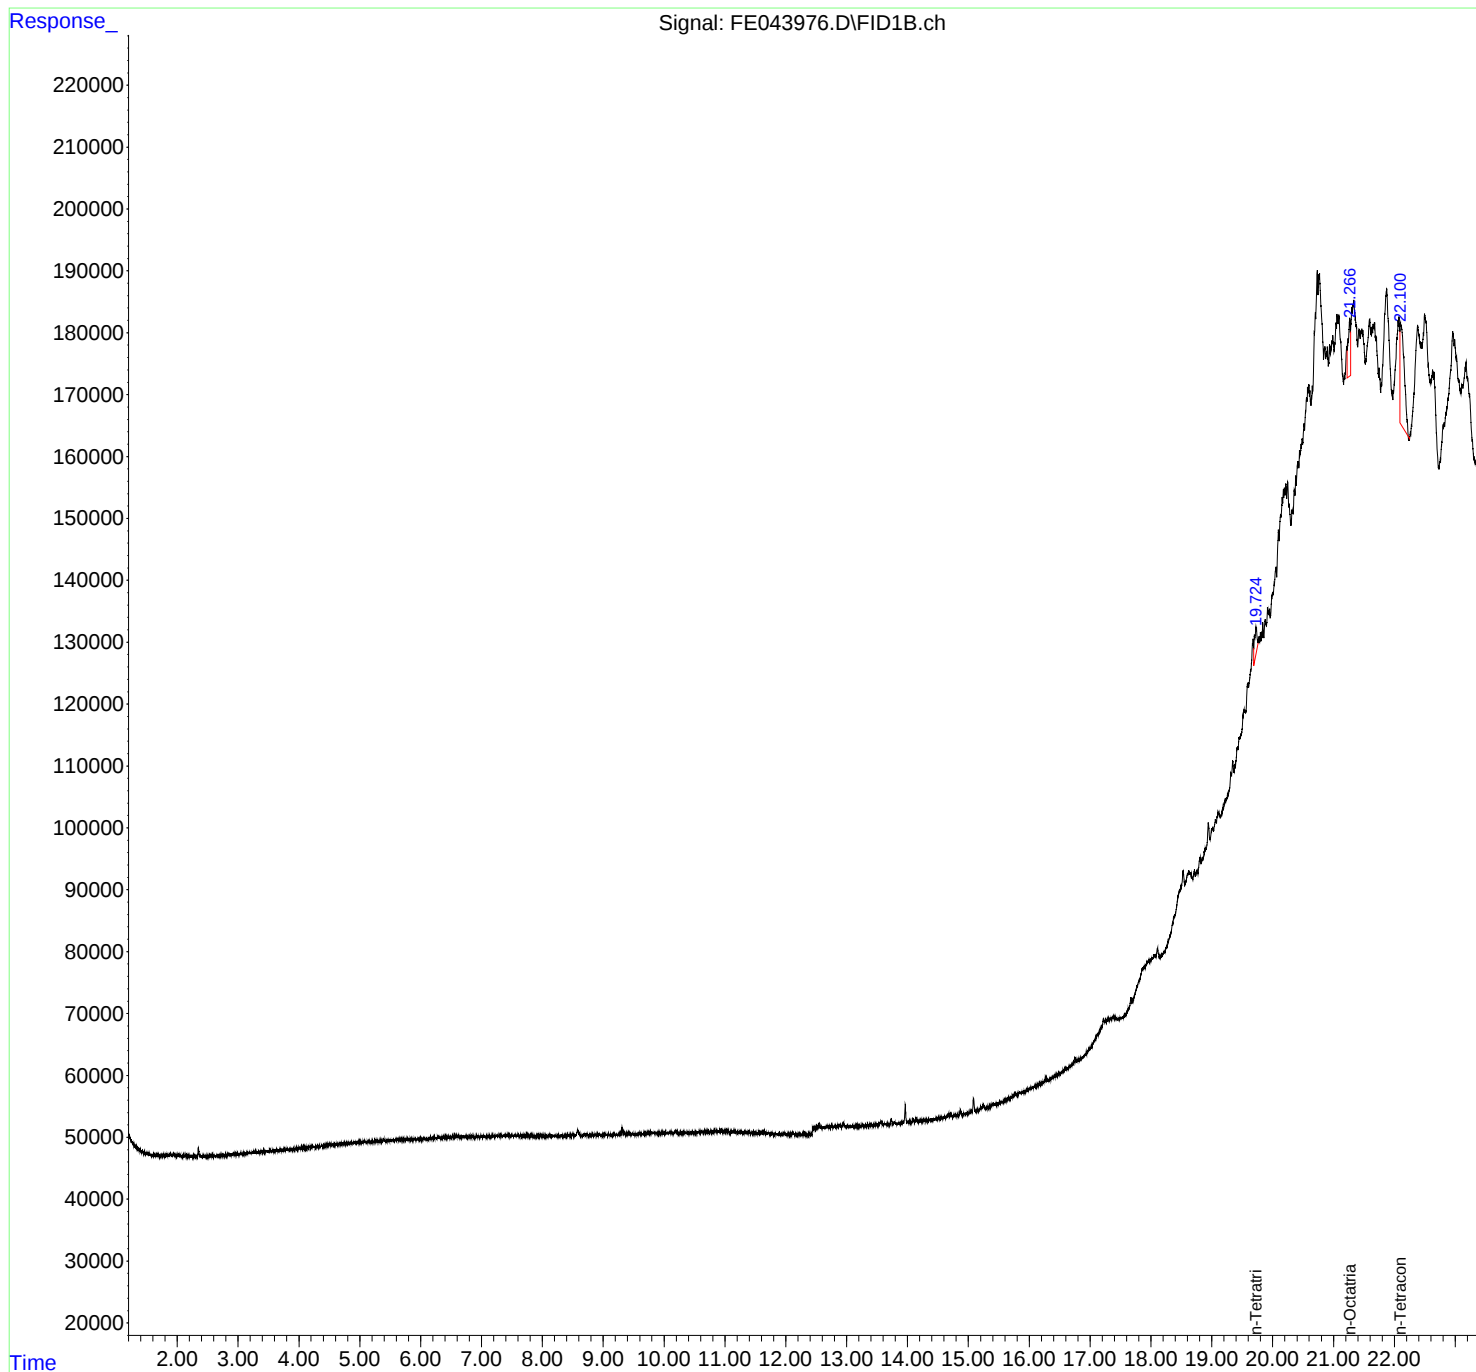


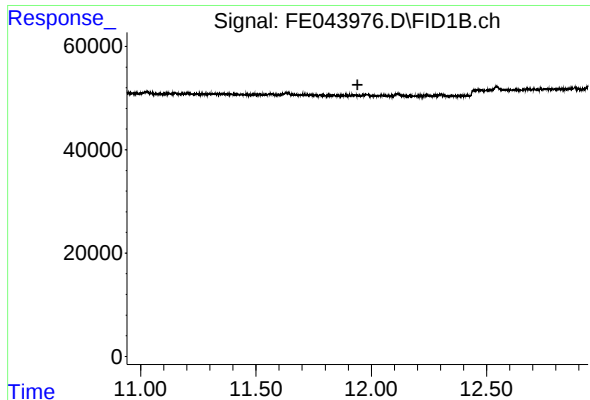

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.940 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

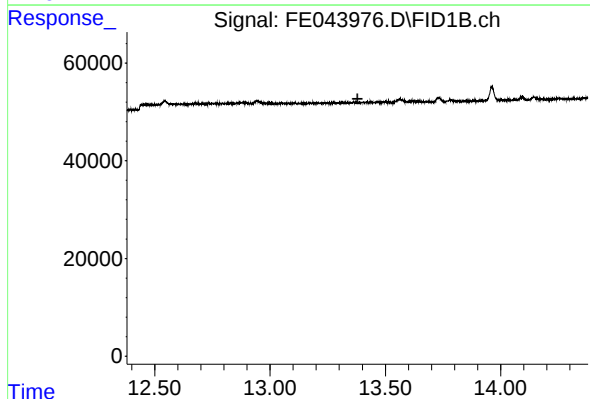


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.379 min
Response: 0
Conc: N.D.

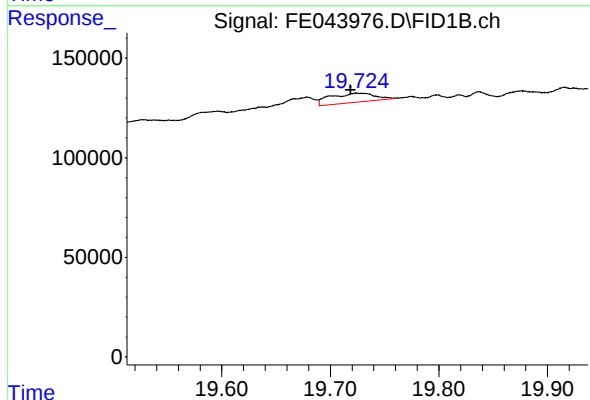


#19 n-Tetratriacontane (C34)

R.T.: 19.724 min
Delta R.T.: 0.005 min
Response: 129861
Conc: 0.87 ug/ml

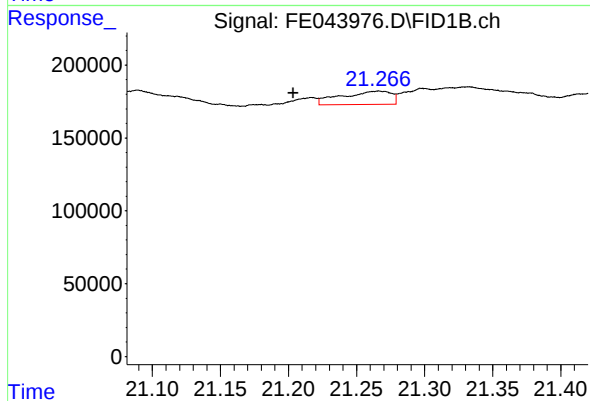

#21 n-Octatriacontane (C38)

R.T.: 21.266 min
Delta R.T.: 0.063 min
Response: 235494
Conc: 1.77 ug/ml

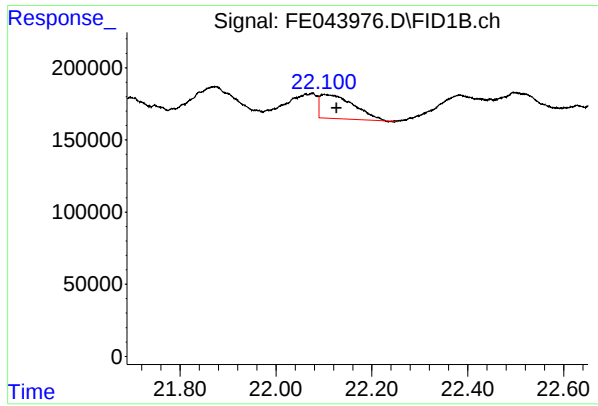

#22 n-Tetracontane (C40)

R.T.: 22.099 min
Delta R.T.: -0.028 min
Response: 786363
Conc: 6.09 ug/ml

Instrument :

FID_E

ClientSampleId :