

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE081524AL\
 Data File : FE049607.D
 Signal(s) : FID1B.ch
 Acq On : 15 Aug 2024 07:29
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 16 01:36:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 081424.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 14 11:05:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) T n-Eicosane (C20)	12.852	152521	1.022 ug/ml
11) T n-Heneicosane (C21)	13.478	287624	1.961 ug/ml
13) T n-Docosane (C22)	14.067	45854	0.315 ug/ml
14) T n-Tetracosane (C24)	15.171	183380	1.261 ug/ml
15) T n-Hexacosane (C26)	16.195	129002	0.894 ug/ml
16) T n-Octacosane (C28)	17.141	160915	1.117 ug/ml
17) T n-Tricontane (C30)	18.028	218450	1.459 ug/ml
18) T n-Dotriacontane (C32)	18.860	287025	1.897 ug/ml
19) T n-Tetratriacontane (C34)	19.640	232298	1.519 ug/ml
20) T n-Hexatriacontane (C36)	20.380	88631	0.584 ug/ml
21) T n-Octatriacontane (C38)	21.108	43589	0.278 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE081524AL\
Data File : FE049607.D
Signal(s) : FID1B.ch
Acq On : 15 Aug 2024 07:29
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 16 01:36:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 081424.M
Quant Title : GC Extractables
QLast Update : Wed Aug 14 11:05:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

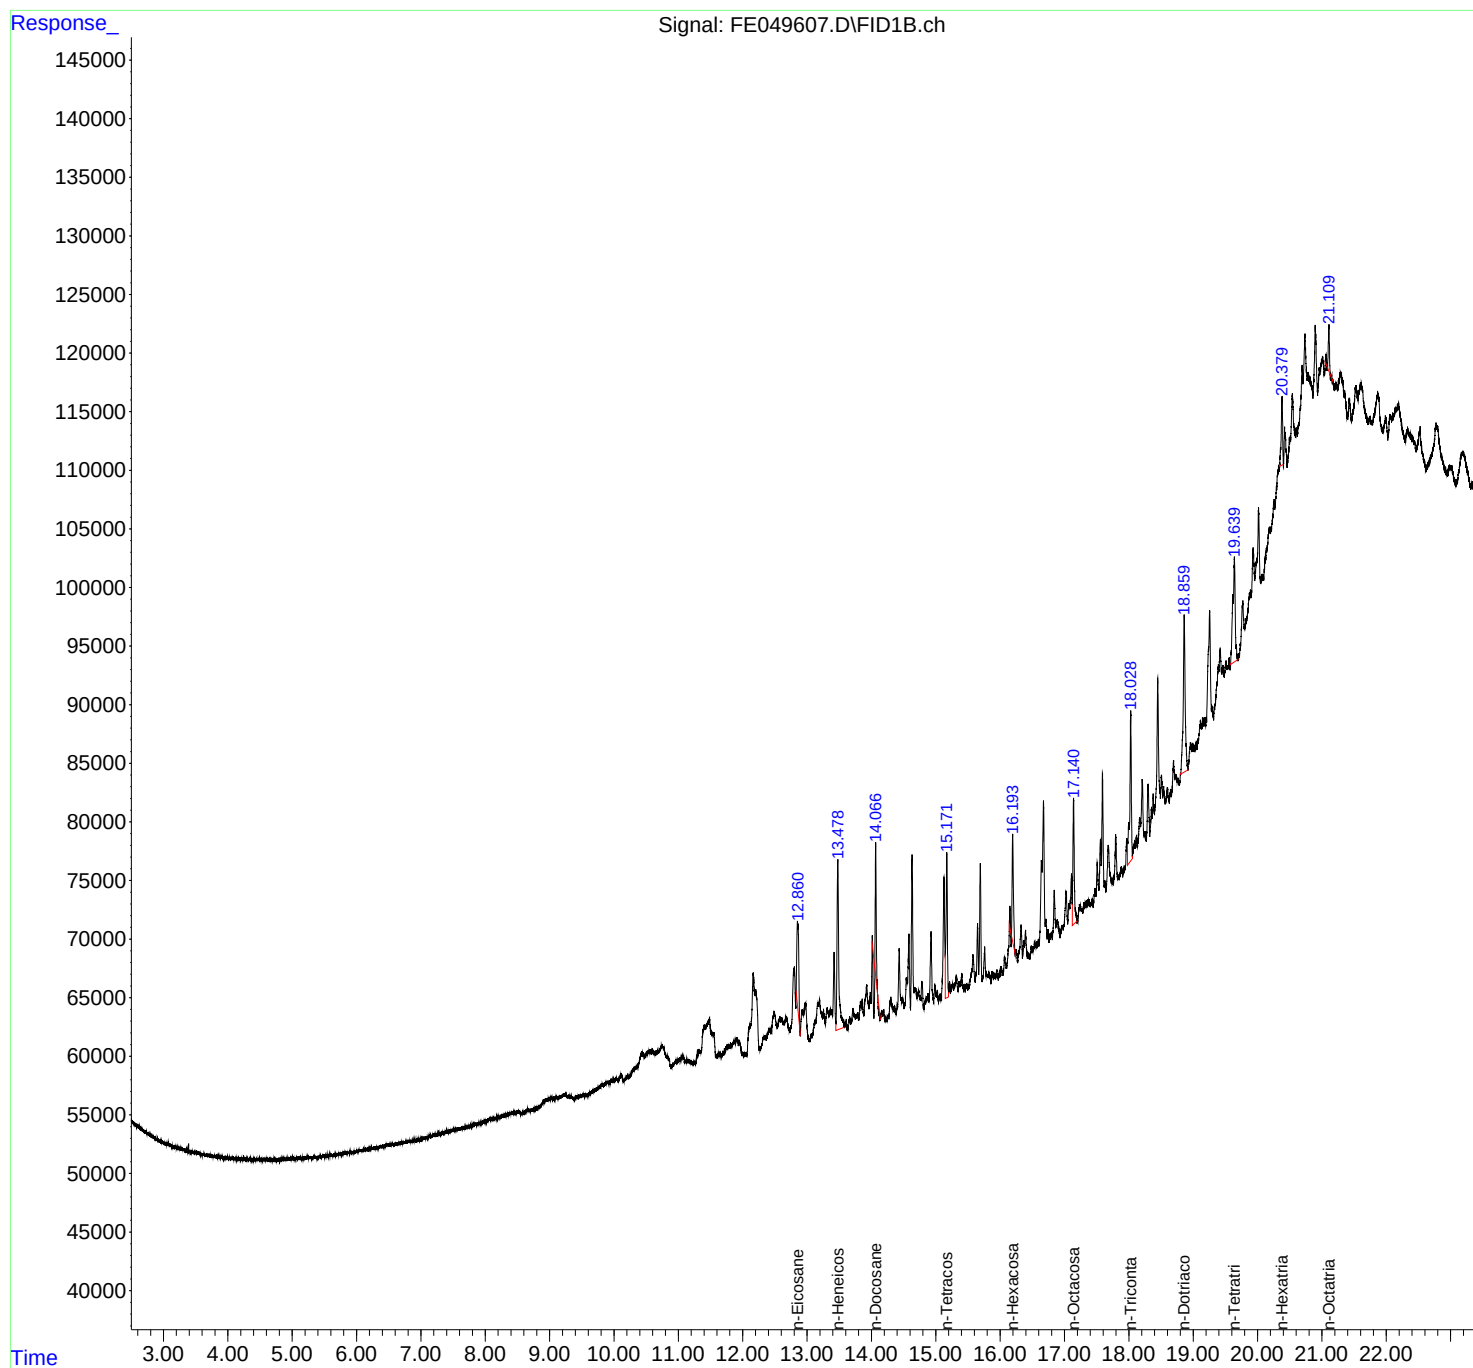


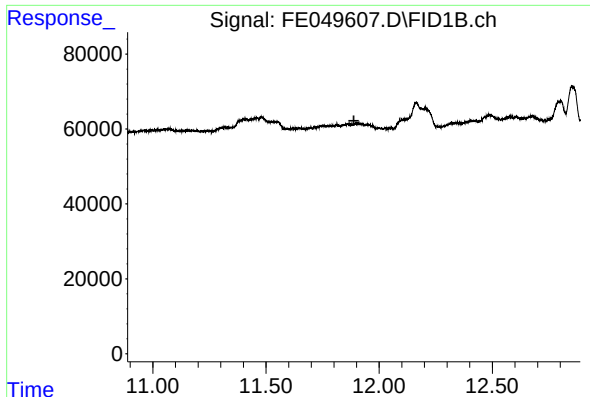

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.888 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

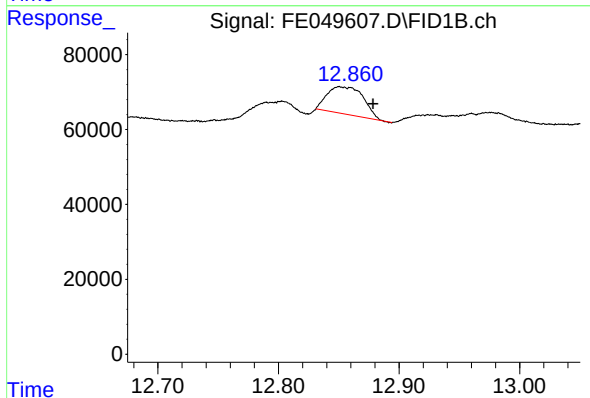


#10 n-Eicosane (C20)

R.T.: 12.852 min
Delta R.T.: -0.027 min
Response: 152521
Conc: 1.02 ug/ml

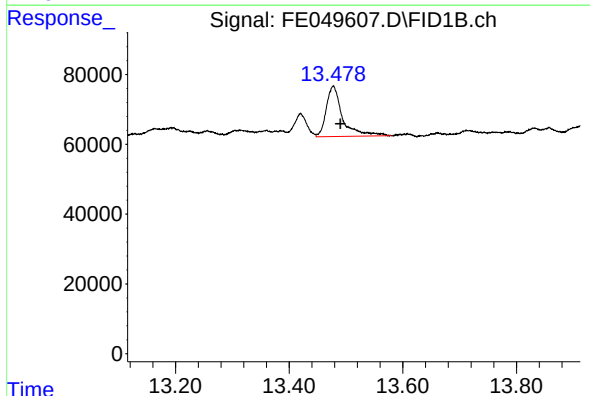


#11 n-Heneicosane (C21)

R.T.: 13.478 min
Delta R.T.: -0.012 min
Response: 287624
Conc: 1.96 ug/ml

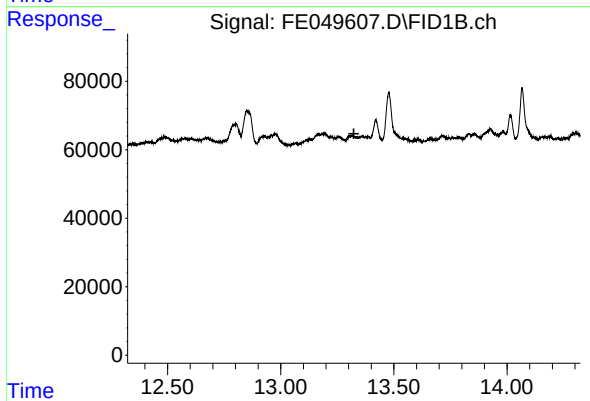

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.323 min
Response: 0
Conc: N.D.

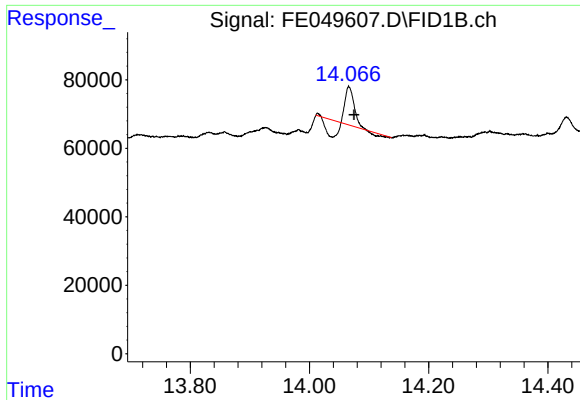

#13 n-Docosane (C22)


R.T.: 14.067 min
Delta R.T.: -0.009 min
Response: 45854
Conc: 0.31 ug/ml

Instrument :
FID_E
ClientSampleId :

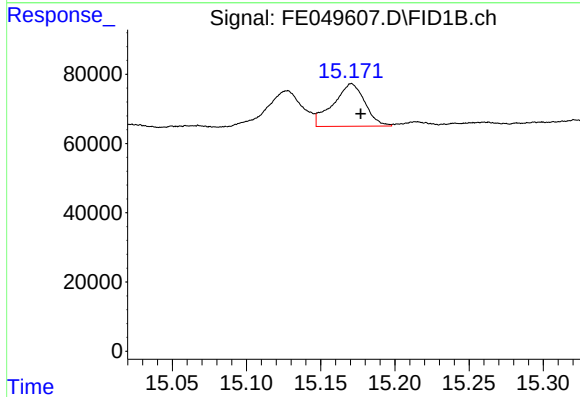


#14 n-Tetracosane (C24)

R.T.: 15.171 min
Delta R.T.: -0.006 min
Response: 183380
Conc: 1.26 ug/ml

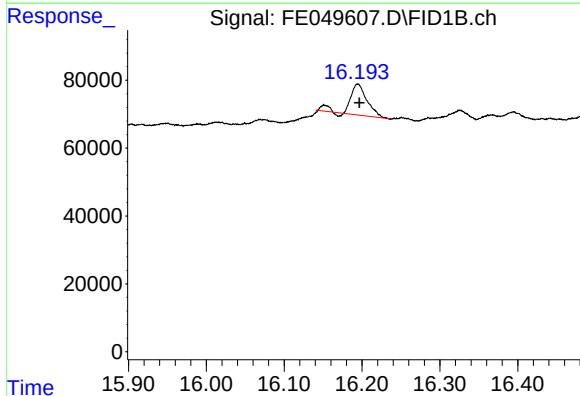


#15 n-Hexacosane (C26)

R.T.: 16.195 min
Delta R.T.: -0.002 min
Response: 129002
Conc: 0.89 ug/ml

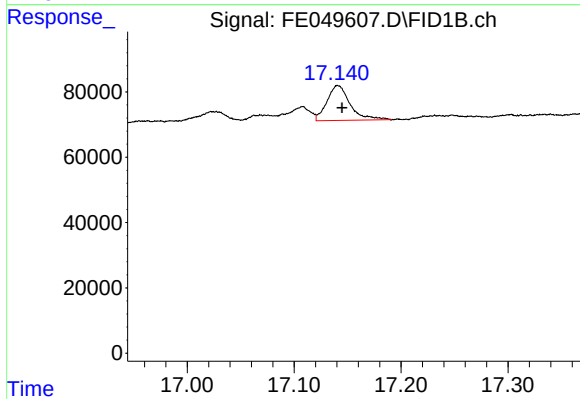

#16 n-Octacosane (C28)


R.T.: 17.141 min
Delta R.T.: -0.004 min
Response: 160915
Conc: 1.12 ug/ml

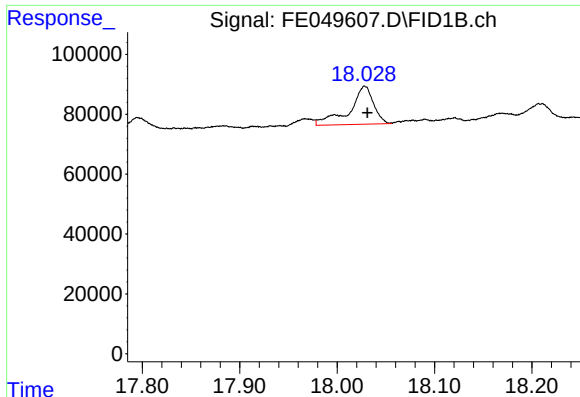

#17 n-Tricontane (C30)


R.T.: 18.028 min
Delta R.T.: -0.003 min
Response: 218450
Conc: 1.46 ug/ml

Instrument :
FID_E
ClientSampleId :

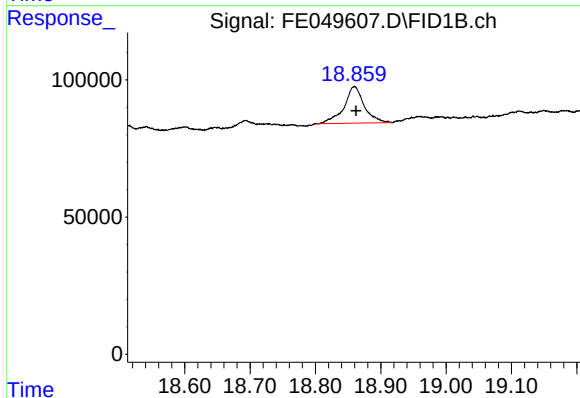


#18 n-Dotriacontane (C32)

R.T.: 18.860 min
Delta R.T.: -0.003 min
Response: 287025
Conc: 1.90 ug/ml

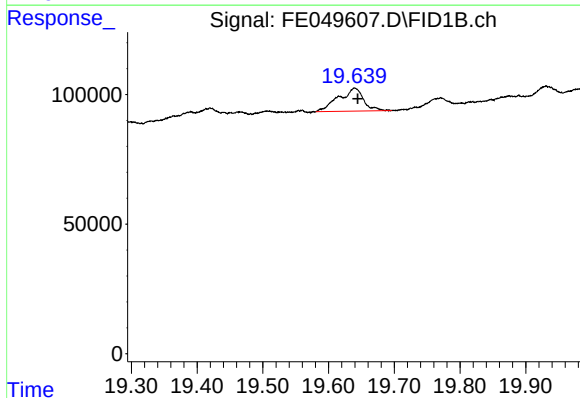


#19 n-Tetratriacontane (C34)

R.T.: 19.640 min
Delta R.T.: -0.004 min
Response: 232298
Conc: 1.52 ug/ml

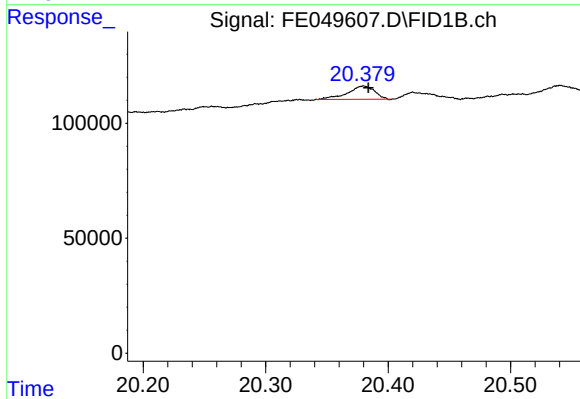

#20 n-Hexatriacontane (C36)

R.T.: 20.380 min
Delta R.T.: -0.004 min
Response: 88631
Conc: 0.58 ug/ml

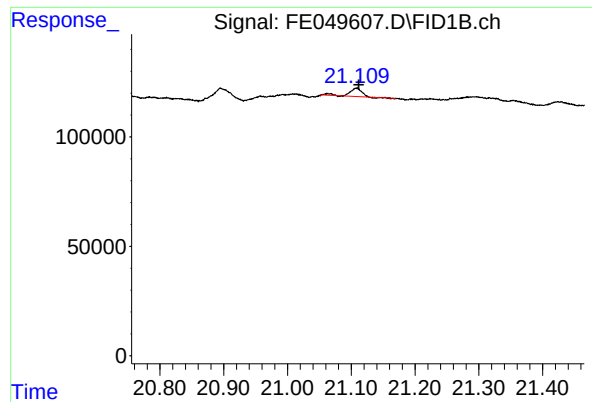

#21 n-Octatriacontane (C38)

R.T.: 21.108 min
Delta R.T.: -0.003 min
Response: 43589
Conc: 0.28 ug/ml

Instrument :

FID_E

ClientSampleId :