

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE081621\
 Data File : FE034172.D
 Signal(s) : FID1B.CH
 Acq On : 16 Aug 2021 23:40
 Operator : DD\AJ
 Sample : M3425-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 17 05:51:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE081621.M
 Quant Title :
 QLast Update : Mon Aug 16 16:04:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.656	6047592	20.586 ug/ml
Target Compounds			
7) N-EICOSANE	12.548	345466	0.975 ug/ml
8) N-DOCOSANE	13.753	376118	1.066 ug/ml
10) N-TETRACOSANE	14.844	2594003	7.515 ug/ml
11) N-HEXACOSANE	15.873	244415	0.729 ug/ml
12) N-OCTACOSANE	16.844	685745	2.109 ug/ml
13) N-TRIACONTANE	17.709	251809	0.817 ug/ml
14) N-DOTRIACONTANE	18.537	358234	1.231 ug/ml
15) N-TETRATRIACONTANE	19.325	188552	0.752 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE081621\
Data File : FE034172.D
Signal(s) : FID1B.CH
Acq On : 16 Aug 2021 23:40
Operator : DD\AJ
Sample : M3425-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 17 05:51:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE081621.M
Quant Title :
QLast Update : Mon Aug 16 16:04:52 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

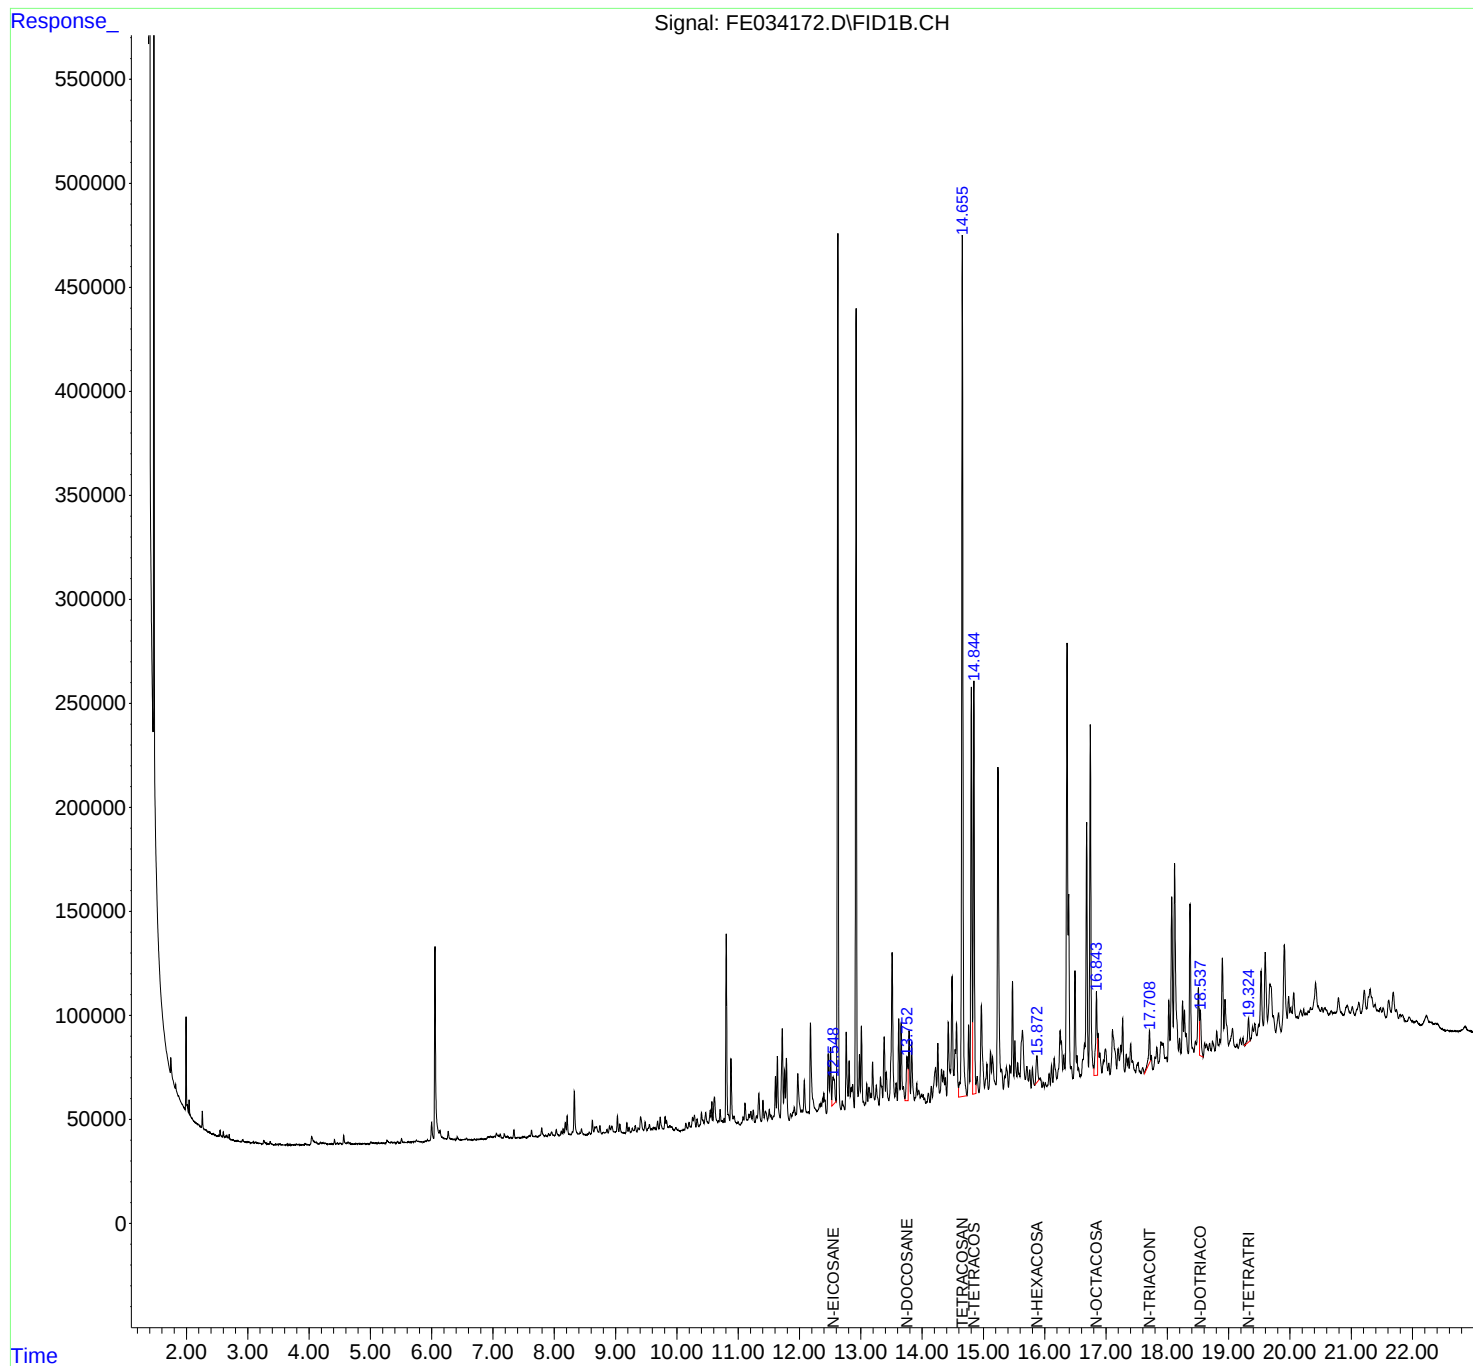


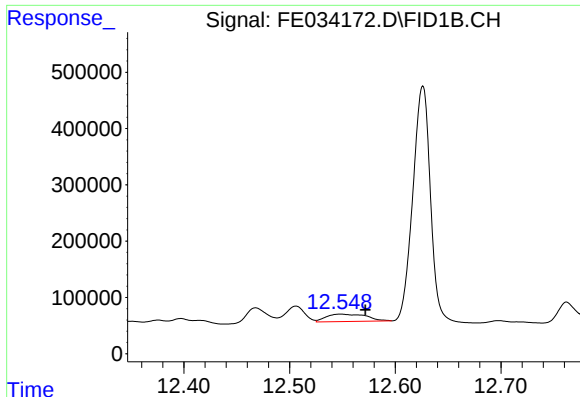

#7 N-EICOSANE


R.T.: 12.548 min
Delta R.T.: -0.024 min
Response: 345466
Conc: 0.97 ug/ml

Instrument :
FID_E
ClientSampleId :

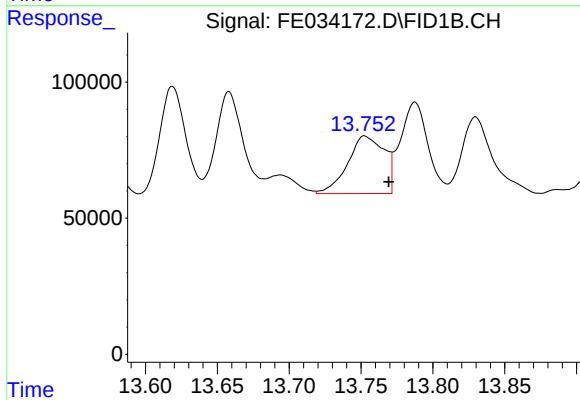


#8 N-DOCOSANE

R.T.: 13.753 min
Delta R.T.: -0.017 min
Response: 376118
Conc: 1.07 ug/ml

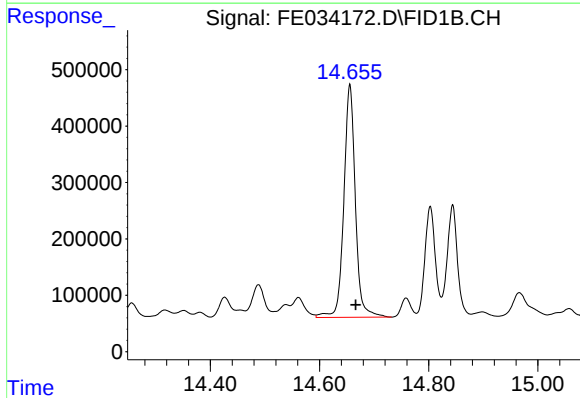


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.656 min
Delta R.T.: -0.011 min
Response: 6047592
Conc: 20.59 ug/ml

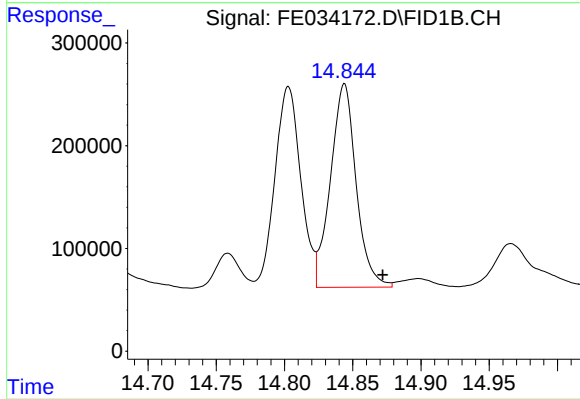

#10 N-TETRACOSANE


R.T.: 14.844 min
Delta R.T.: -0.028 min
Response: 2594003
Conc: 7.51 ug/ml

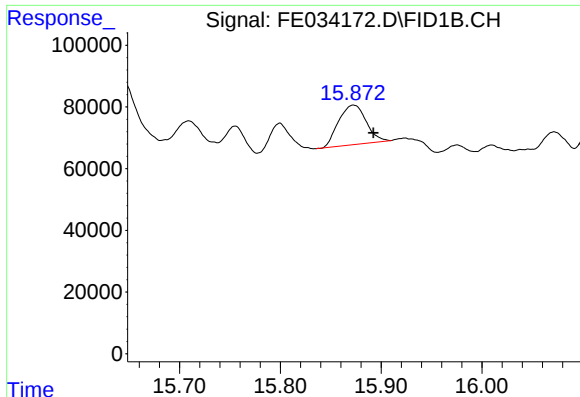

#11 N-HEXACOSANE


R.T.: 15.873 min
Delta R.T.: -0.020 min
Response: 244415
Conc: 0.73 ug/ml

Instrument :
FID_E
ClientSampleId :

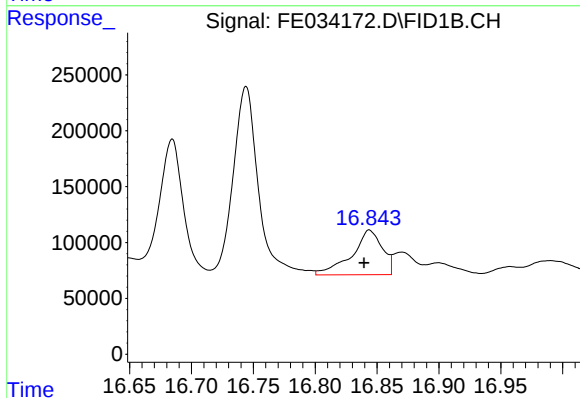


#12 N-OCTACOSANE

R.T.: 16.844 min
Delta R.T.: 0.004 min
Response: 685745
Conc: 2.11 ug/ml

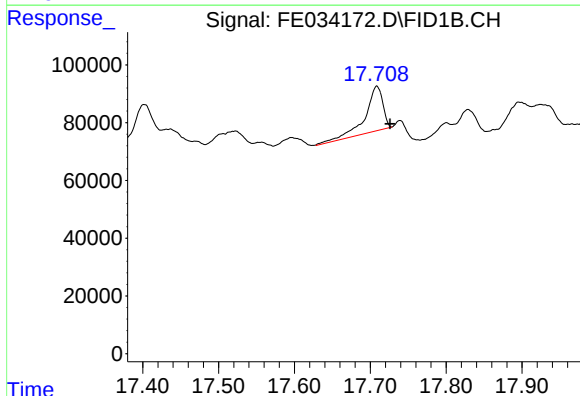


#13 N-TRIACONTANE

R.T.: 17.709 min
Delta R.T.: -0.017 min
Response: 251809
Conc: 0.82 ug/ml

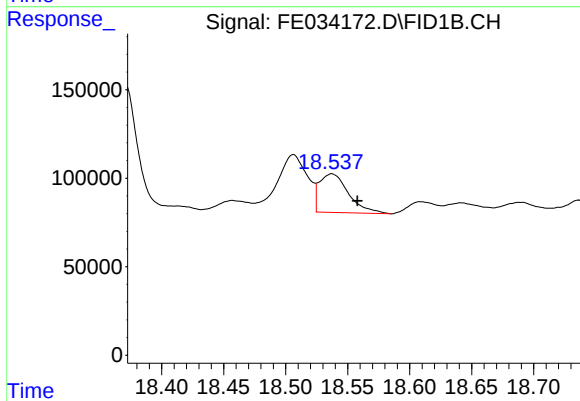

#14 N-DOTRIACONTANE

R.T.: 18.537 min
Delta R.T.: -0.021 min
Response: 358234
Conc: 1.23 ug/ml

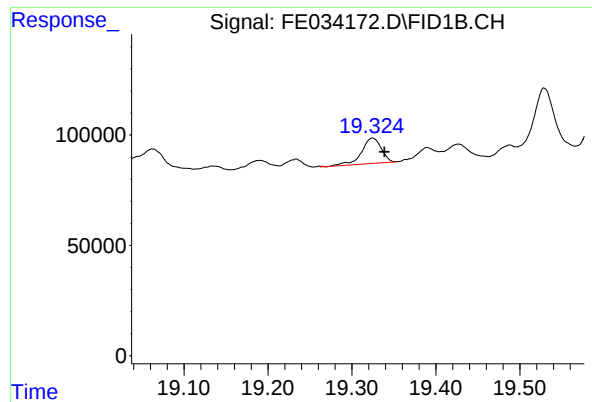

#15 N-TETRATRIACONTANE

R.T.: 19.325 min
Delta R.T.: -0.014 min
Response: 188552
Conc: 0.75 ug/ml

Instrument :
FID_E
ClientSampleId :