

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE081621\  
 Data File : FE034177.D  
 Signal(s) : FID1B.CH  
 Acq On : 17 Aug 2021 2:33  
 Operator : DD\AJ  
 Sample : M3425-17  
 Misc :  
 ALS Vial : 21 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Aug 17 05:52:48 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE081621.M  
 Quant Title :  
 QLast Update : Mon Aug 16 16:04:52 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.    | Response | Conc Units   |
|-------------------------------|---------|----------|--------------|
| -----                         |         |          |              |
| System Monitoring Compounds   |         |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.653  | 5726915  | 19.494 ug/ml |
| Target Compounds              |         |          |              |
| 7) N-EICOSANE                 | 12.622f | 1007216  | 2.842 ug/ml  |
| 10) N-TETRACOSANE             | 14.843  | 579648   | 1.679 ug/ml  |
| -----                         |         |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE081621\  
Data File : FE034177.D  
Signal(s) : FID1B.CH  
Acq On : 17 Aug 2021 2:33  
Operator : DD\AJ  
Sample : M3425-17  
Misc :  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Aug 17 05:52:48 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE081621.M  
Quant Title :  
QLast Update : Mon Aug 16 16:04:52 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

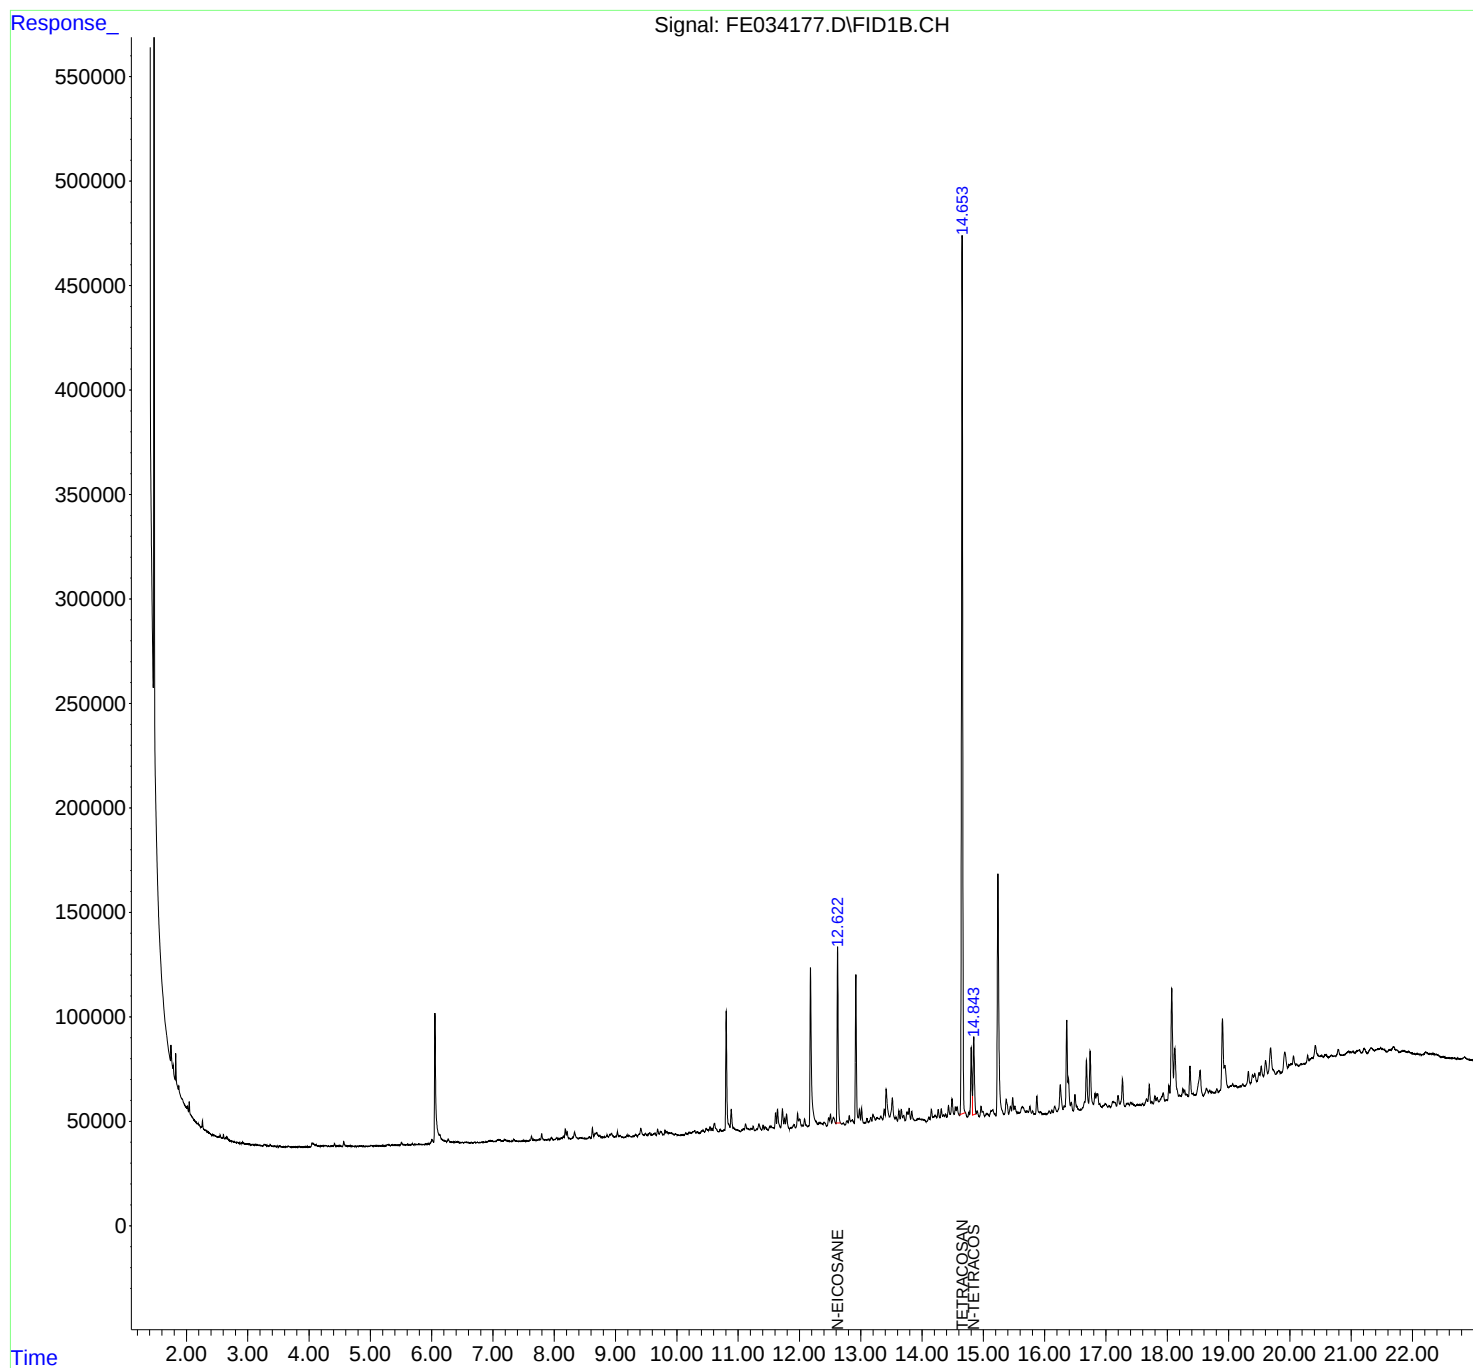


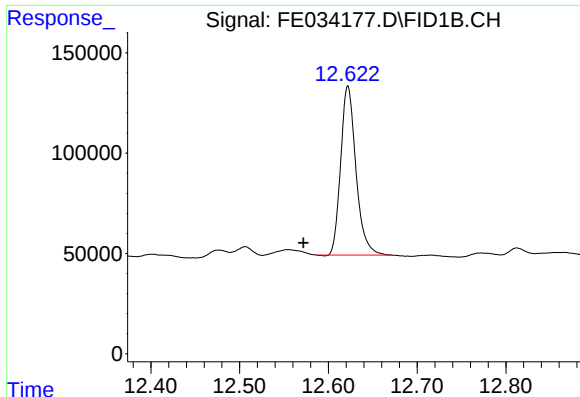

#7 N-EICOSANE


R.T.: 12.622 min  
Delta R.T.: 0.050 min  
Response: 1007216  
Conc: 2.84 ug/ml

Instrument :  
FID\_E  
ClientSampleId :

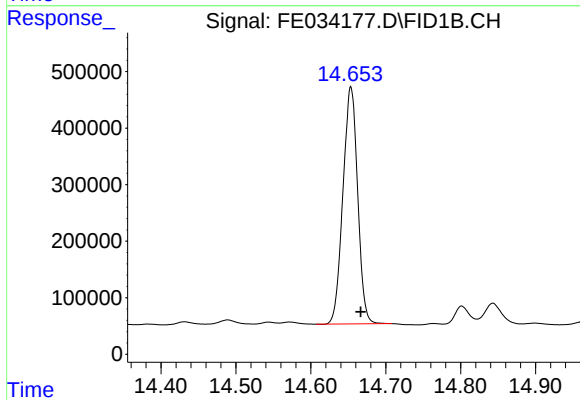

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.653 min  
Delta R.T.: -0.013 min  
Response: 5726915  
Conc: 19.49 ug/ml

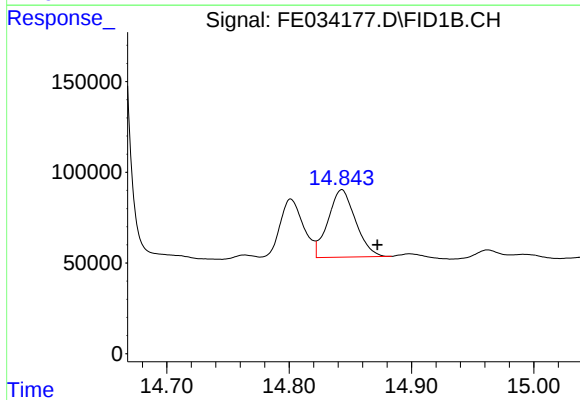

#10 N-TETRACOSANE

R.T.: 14.843 min  
Delta R.T.: -0.029 min  
Response: 579648  
Conc: 1.68 ug/ml