

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE081621\  
Data File : FE034167.D  
Signal(s) : FID1B.CH  
Acq On : 16 Aug 2021 20:47  
Operator : DD\AJ  
Sample : M3424-08  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
19N

Manual Integrations  
APPROVED

mohammad  
8/17/2021 3:45:28 PM

Integration File: autoint1.e  
Quant Time: Aug 17 05:50:43 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE081621.M  
Quant Title :  
QLast Update : Mon Aug 16 16:04:52 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units    |
|-------------------------------|--------|----------|---------------|
| -----                         |        |          |               |
| System Monitoring Compounds   |        |          |               |
| 9) S TETRACOSANE-d50 (SURR... | 14.655 | 6168424  | 20.997 ug/mlm |
| Target Compounds              |        |          |               |
| -----                         |        |          |               |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE081621\  
Data File : FE034167.D  
Signal(s) : FID1B.CH  
Acq On : 16 Aug 2021 20:47  
Operator : DD\AJ  
Sample : M3424-08  
Misc :  
ALS Vial : 13 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
19N


Manual Integrations  
APPROVED

mohammad  
8/17/2021 3:45:28 PM

Integration File: autoint1.e  
Quant Time: Aug 17 05:50:43 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE081621.M  
Quant Title :  
QLast Update : Mon Aug 16 16:04:52 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

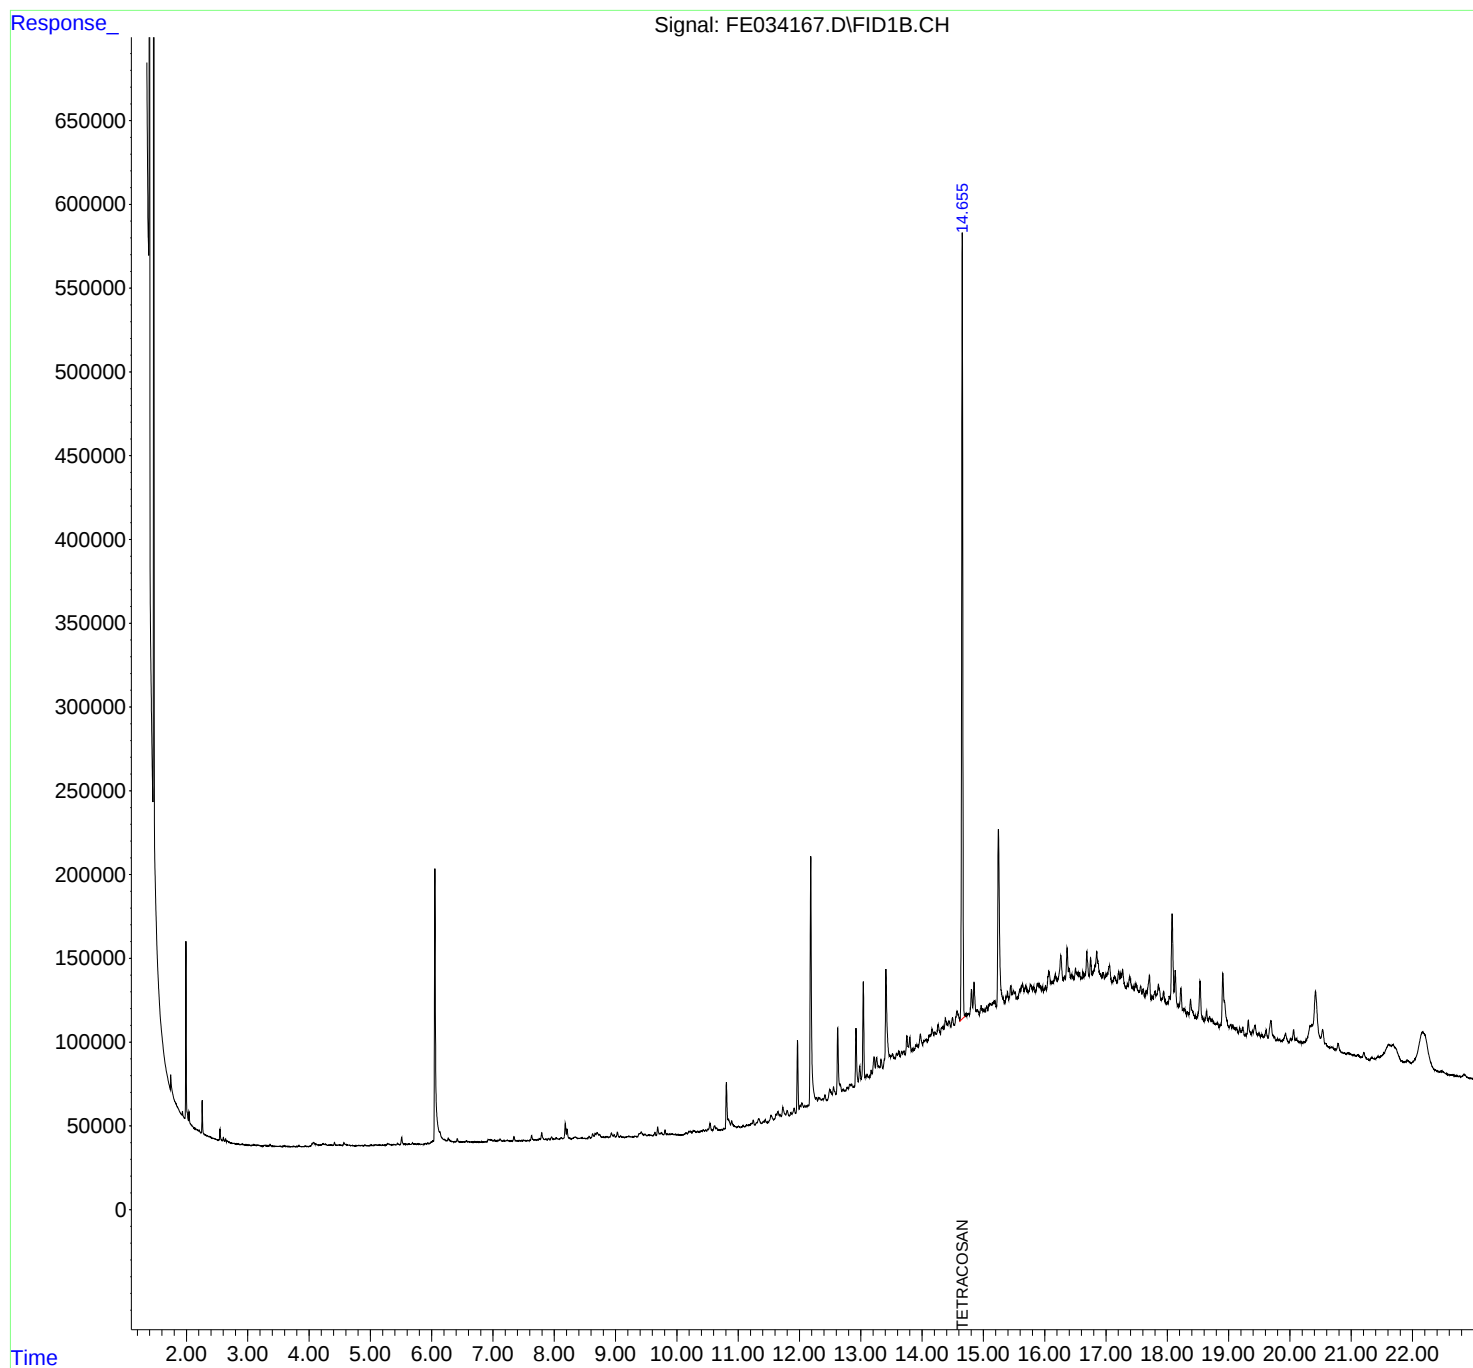

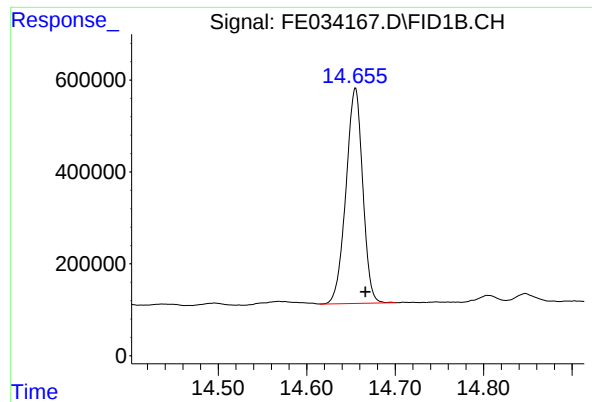

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.655 min  
Delta R.T.: -0.012 min  
Response: 6168424  
Conc: 21.00 ug/ml m

Instrument :  
FID\_E  
ClientSampleId :  
19N

Manual Integrations  
APPROVED

mohammad  
8/17/2021 3:45:28 PM