

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE081621\
Data File : FE034178.D
Signal(s) : FID1B.CH
Acq On : 17 Aug 2021 3:07
Operator : DD\AJ
Sample : M3425-20
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
23S

Integration File: autoint1.e
Quant Time: Aug 17 05:52:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE081621.M
Quant Title :
QLast Update : Mon Aug 16 16:04:52 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.654	6037750	20.552 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE081621\
Data File : FE034178.D
Signal(s) : FID1B.CH
Acq On : 17 Aug 2021 3:07
Operator : DD\AJ
Sample : M3425-20
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
23S

Integration File: autoint1.e
Quant Time: Aug 17 05:52:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE081621.M
Quant Title :
QLast Update : Mon Aug 16 16:04:52 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

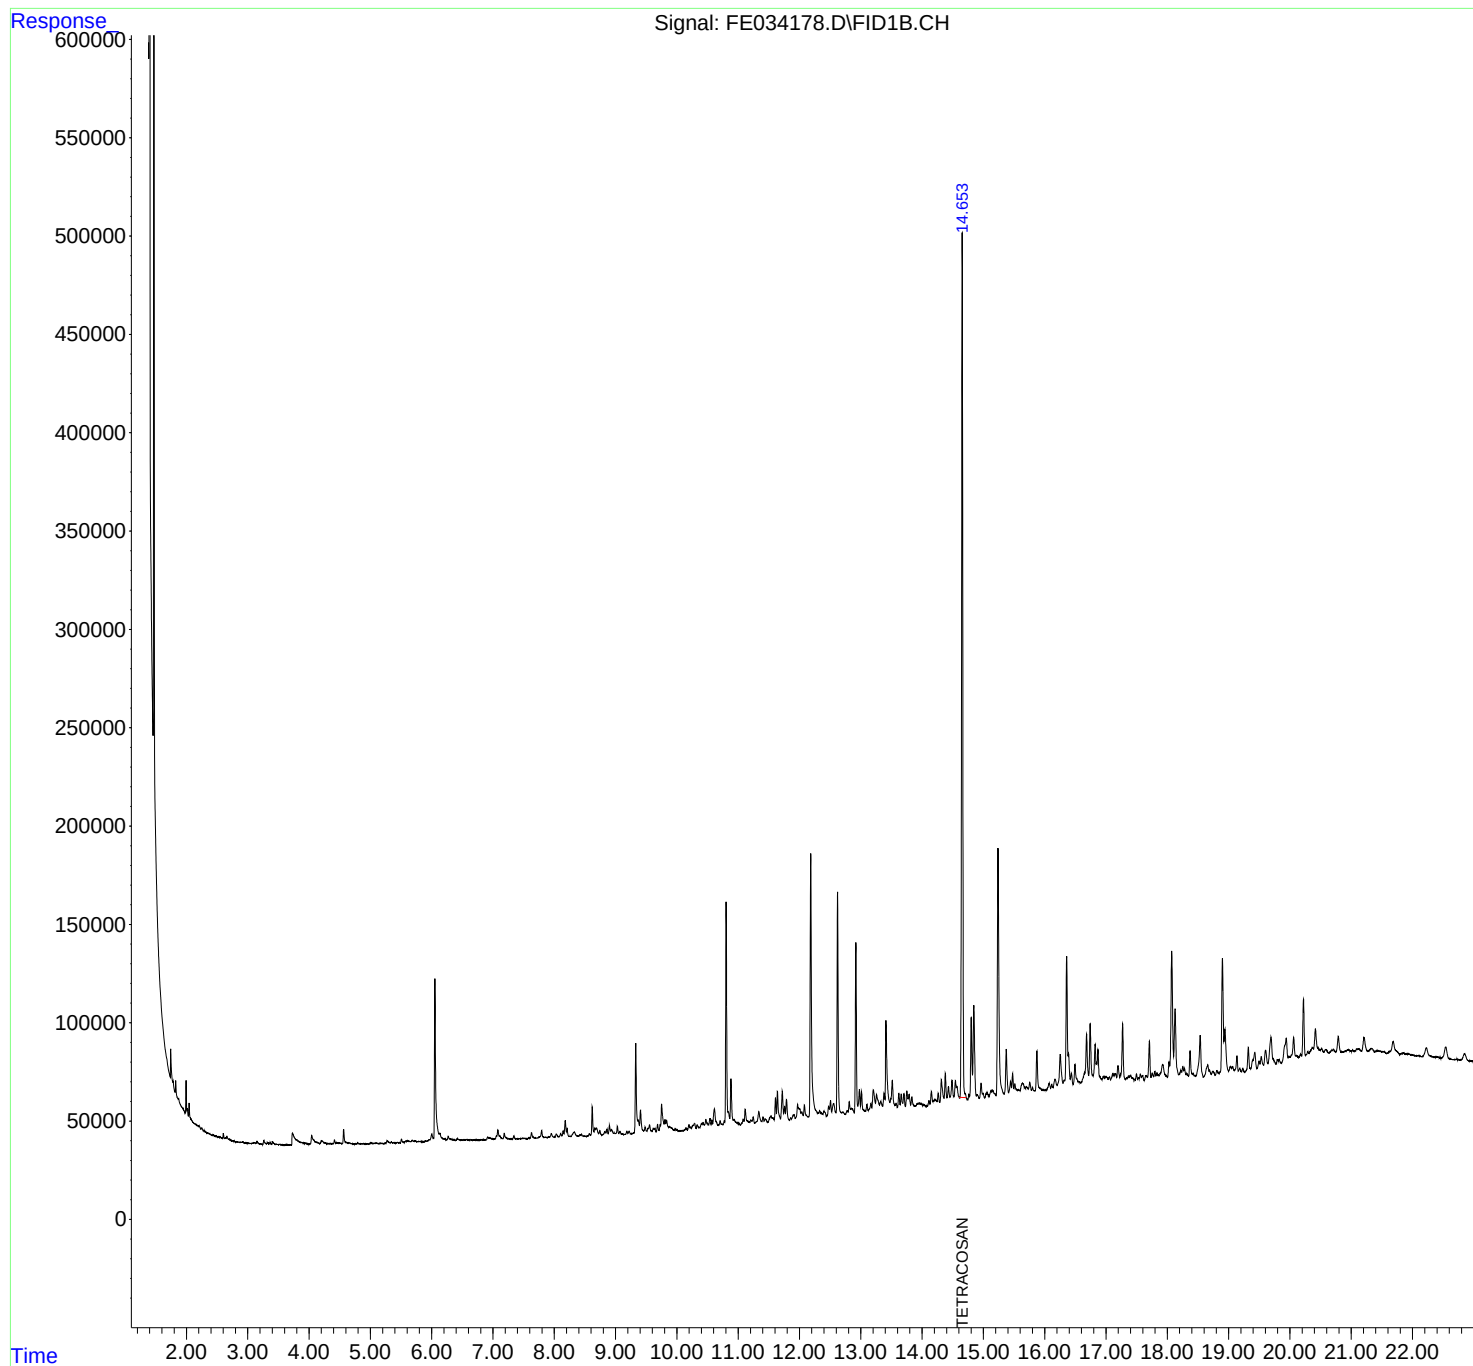

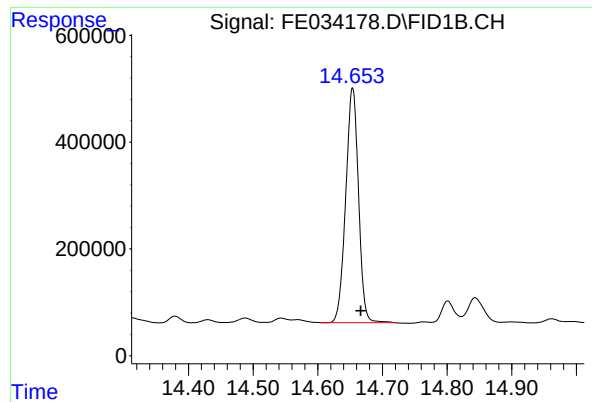

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.654 min
Delta R.T.: -0.013 min
Response: 6037750
Conc: 20.55 ug/ml

Instrument :
FID_E
ClientSampleId :
23S