

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE081825AL\
Data File : FE055350.D
Signal(s) : FID1B.ch
Acq On : 18 Aug 2025 08:49
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 18 14:25:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 080125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 13:47:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	18.248	119525	0.971 ug/ml
18) T	n-Dotriacontane (C32)	19.082	197951	1.622 ug/ml
19) T	n-Tetratriacontane (C34)	19.866	143381	1.226 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE081825AL\
Data File : FE055350.D
Signal(s) : FID1B.ch
Acq On : 18 Aug 2025 08:49
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 18 14:25:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 080125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 13:47:09 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

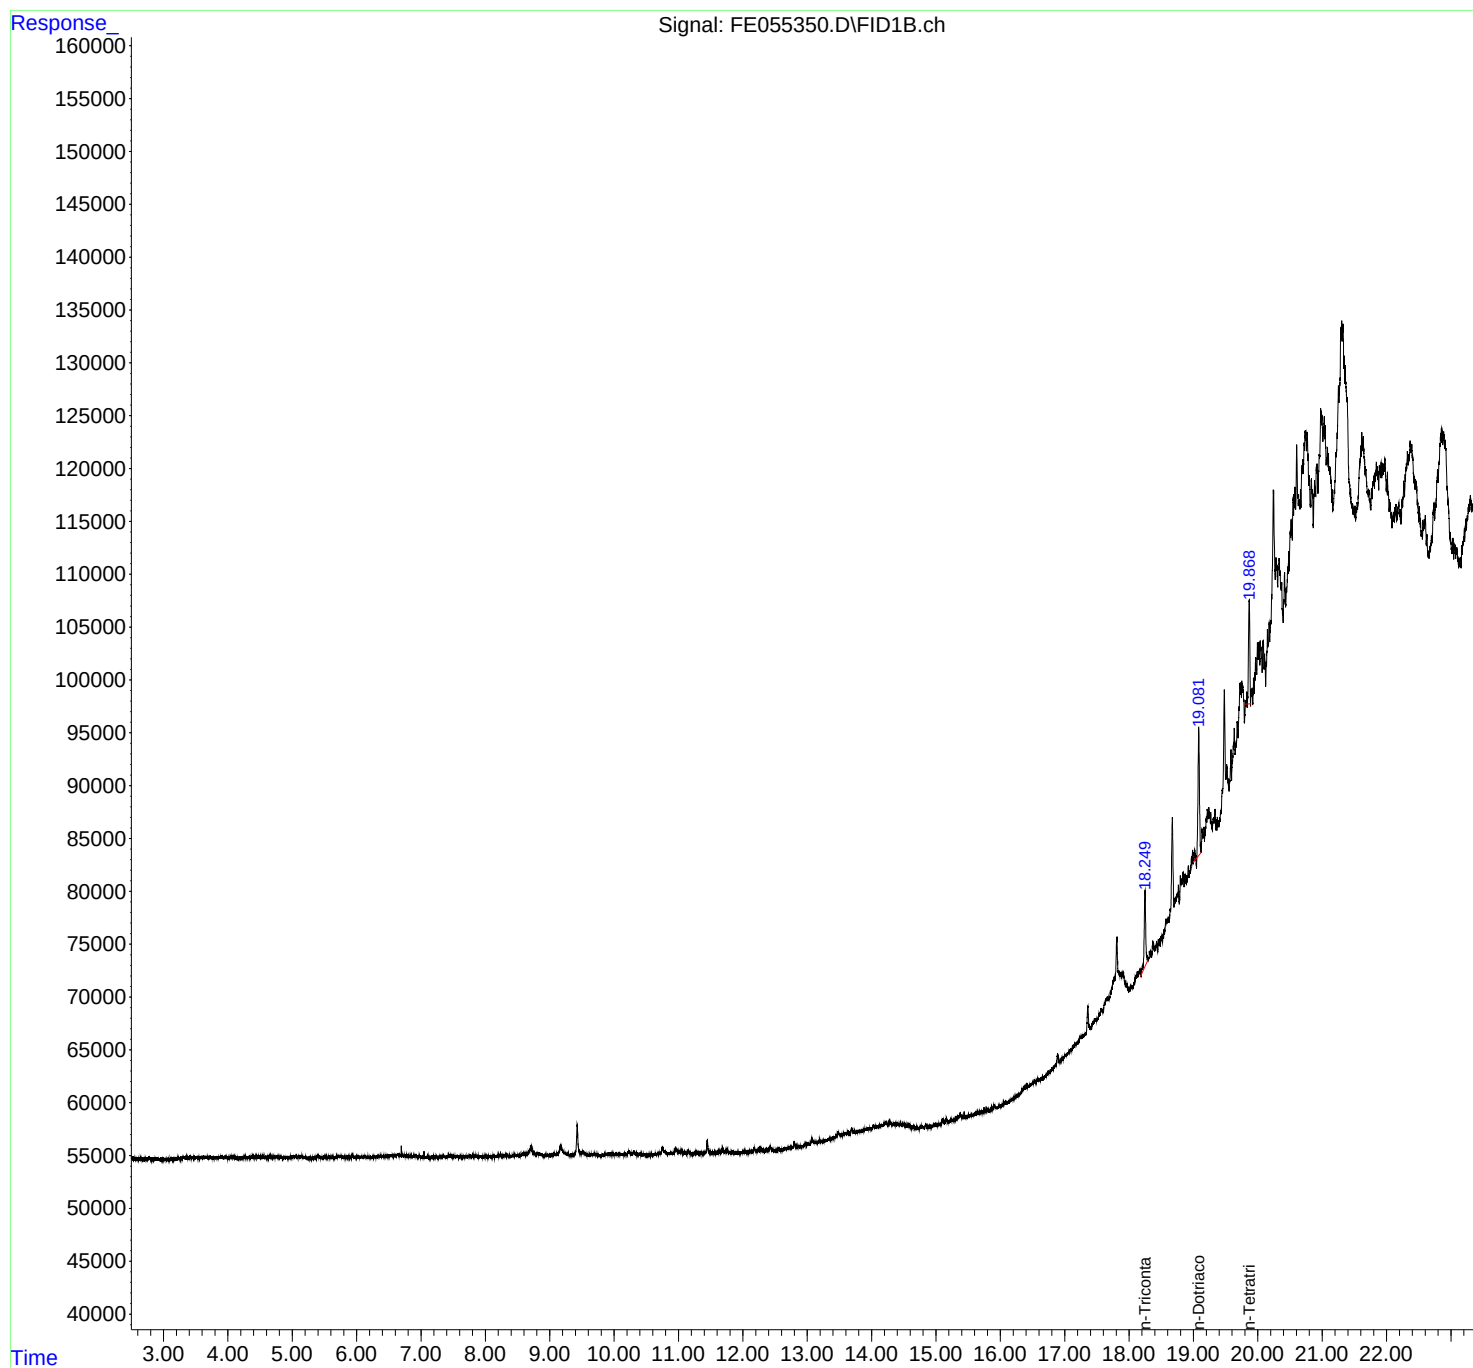


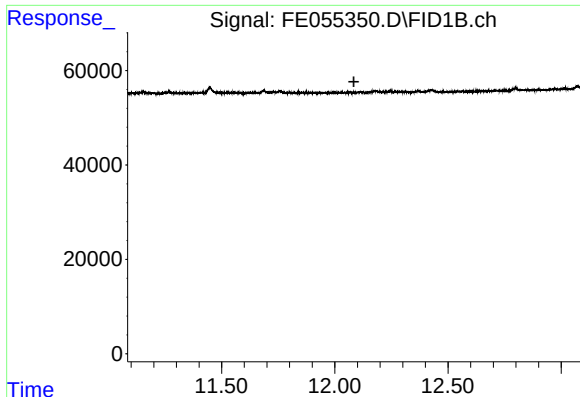

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 12.084 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

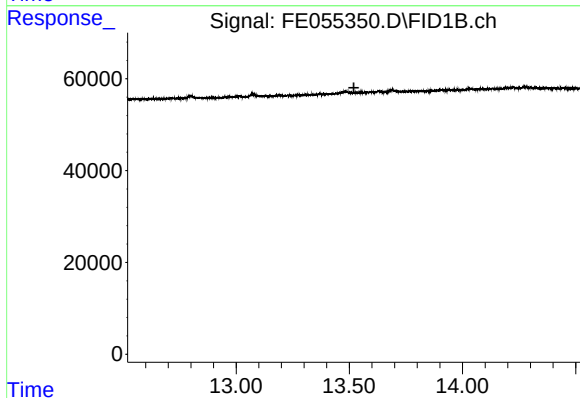


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.520 min
Response: 0
Conc: N.D.

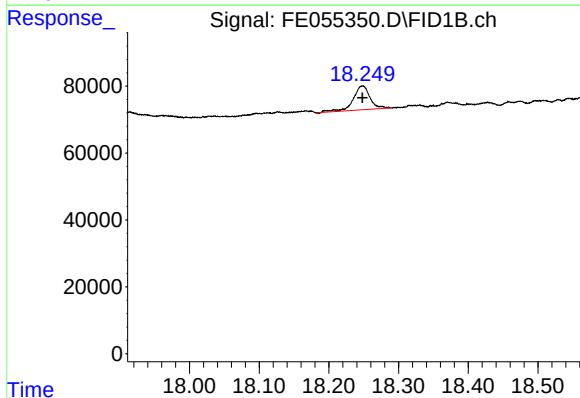


#17 n-Tricontane (C30)

R.T.: 18.248 min
Delta R.T.: 0.000 min
Response: 119525
Conc: 0.97 ug/ml

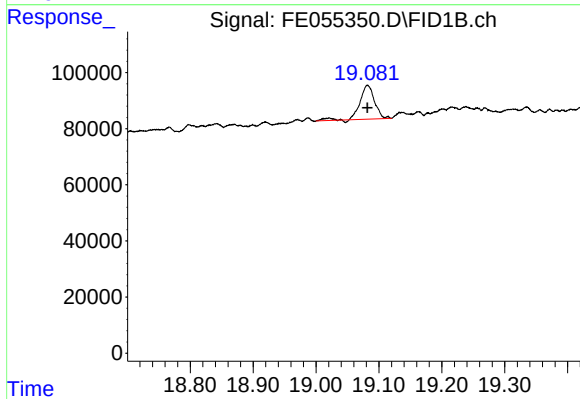

#18 n-Dotriacontane (C32)

R.T.: 19.082 min
Delta R.T.: 0.000 min
Response: 197951
Conc: 1.62 ug/ml

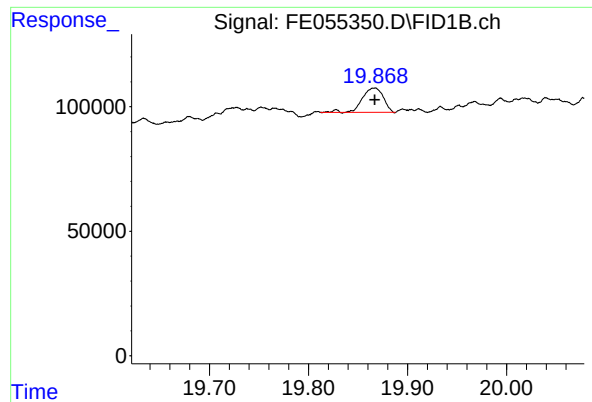

#19 n-Tetratriacontane (C34)

R.T.: 19.866 min
Delta R.T.: 0.000 min
Response: 143381
Conc: 1.23 ug/ml

Instrument :
FID_E
ClientSampleId :