

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE081919\
 Data File : FE030255.D
 Signal(s) : FID1B.CH
 Acq On : 20 Aug 2019 2:33
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 20 04:01:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE080919.M
 Quant Title :
 QLast Update : Fri Aug 09 14:35:21 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.575	3519694	18.066 ug/ml
Target Compounds				
12)	N-DOTRIACONTANE	18.468	53940	0.295 ug/ml
14)	N-HEXATRIACONTANE	19.997	860739	5.120 ug/ml
15)	N-TETRACONTANE	21.535	277948	1.783 ug/ml
16)	N-TETRTETRACOCTANE	24.121	18797	0.127 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE081919\
Data File : FE030255.D
Signal(s) : FID1B.CH
Acq On : 20 Aug 2019 2:33
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 20 04:01:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE080919.M
Quant Title :
QLast Update : Fri Aug 09 14:35:21 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 uL
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

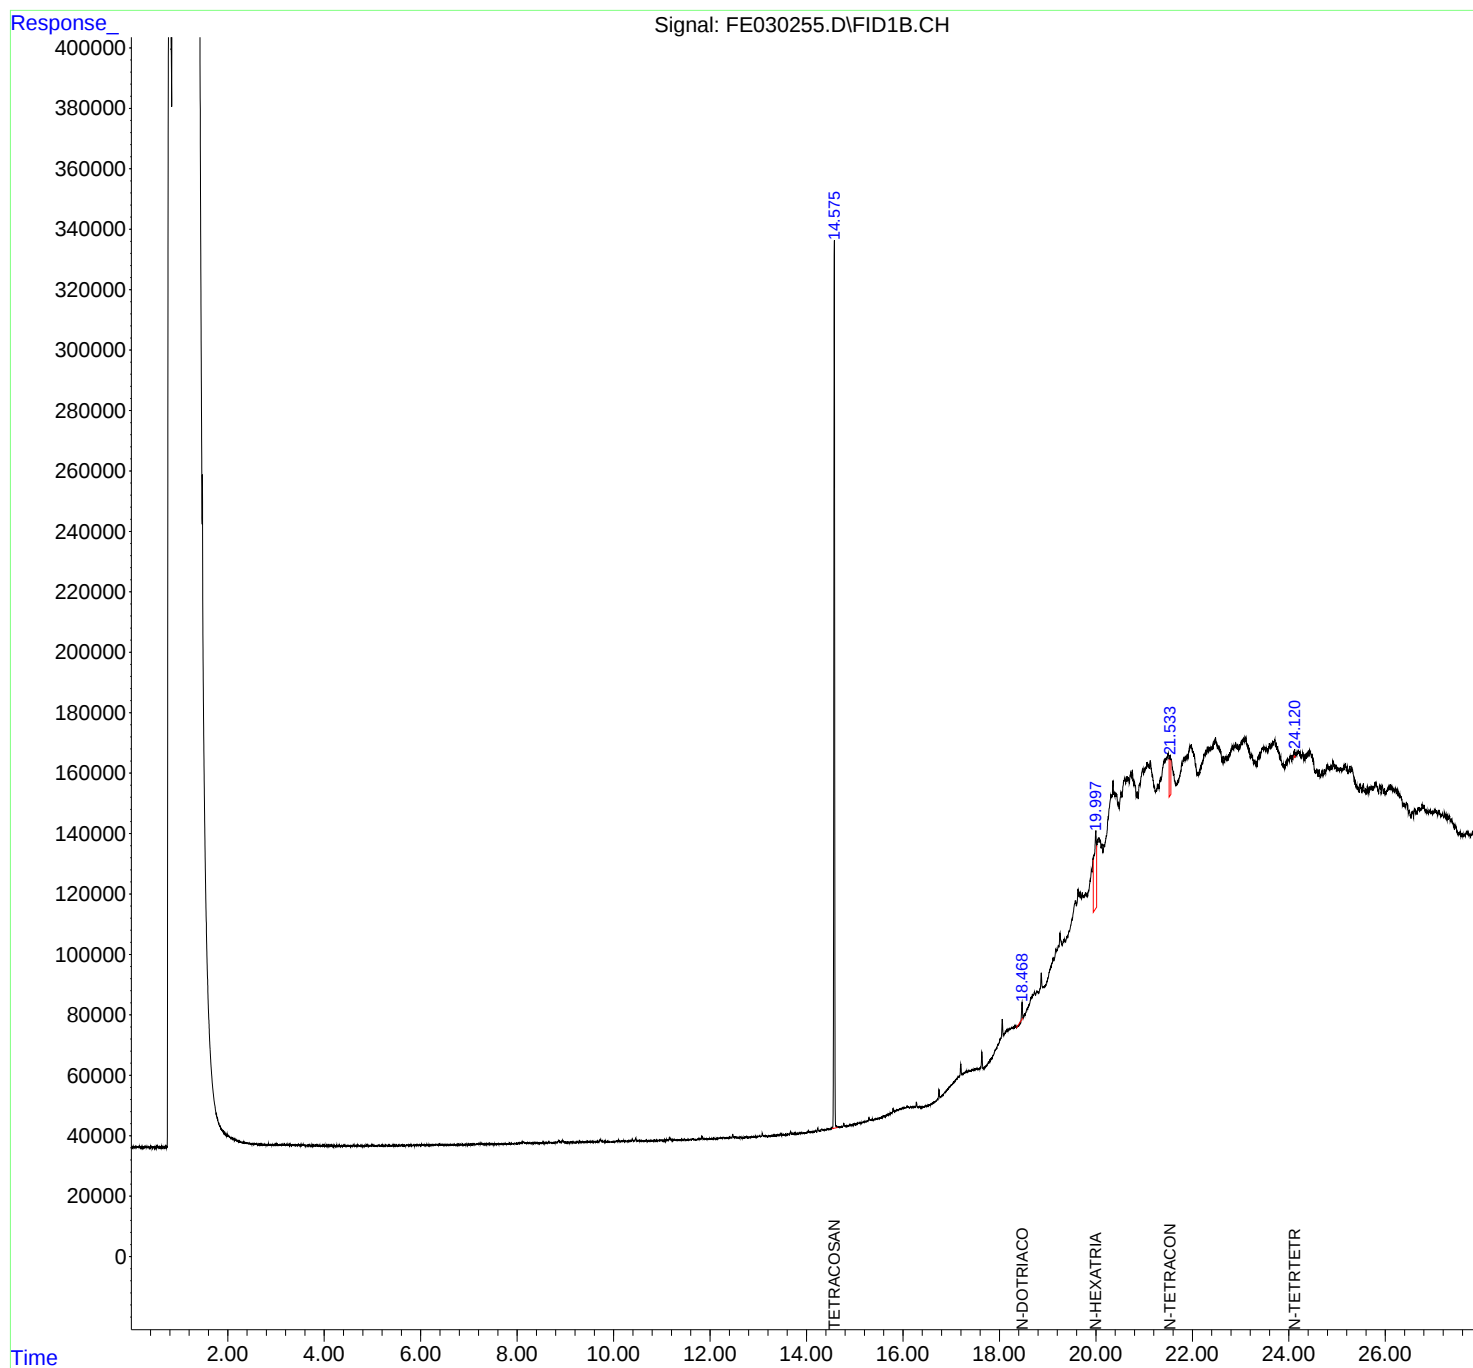

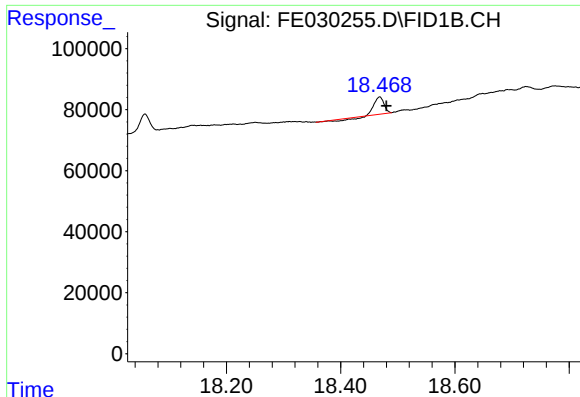


#12 N-DOTRIACONTANE

R.T.: 18.468 min
Delta R.T.: -0.012 min
Response: 53940
Conc: 0.30 ug/ml

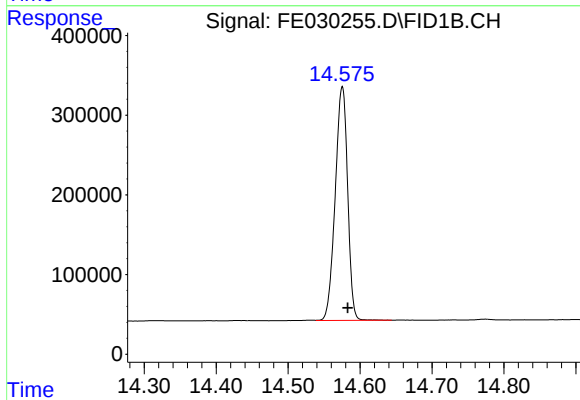


#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.575 min
Delta R.T.: -0.007 min
Response: 3519694
Conc: 18.07 ug/ml

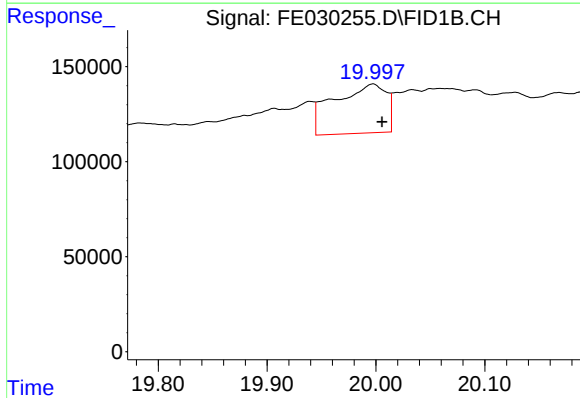


#14 N-HEXATRIACONTANE

R.T.: 19.997 min
Delta R.T.: -0.008 min
Response: 860739
Conc: 5.12 ug/ml

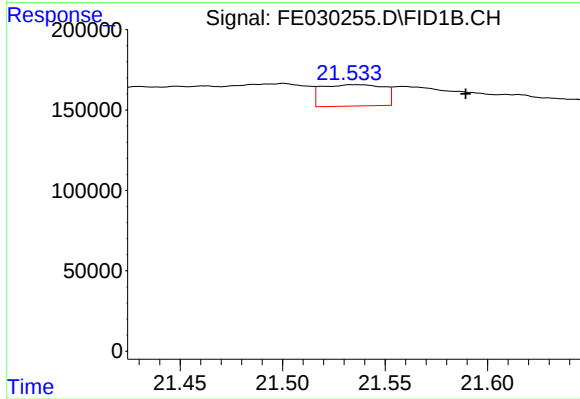

#15 N-TETRACONTANE

R.T.: 21.535 min
Delta R.T.: -0.055 min
Response: 277948
Conc: 1.78 ug/ml

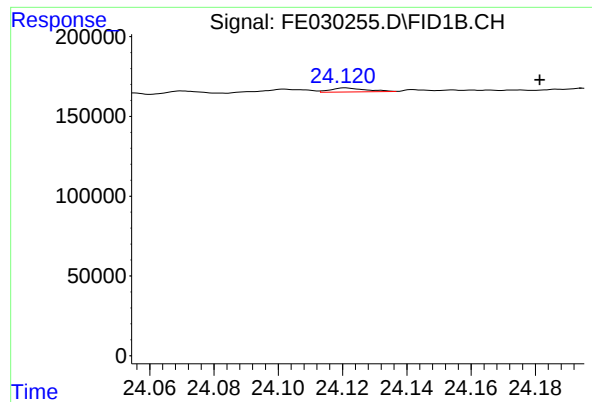

#16 N-TETRTETRACOCTANE

R.T.: 24.121 min

Delta R.T.: -0.060 min

Response: 18797

Conc: 0.13 ug/ml