

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082021\
Data File : FE034199.D
Signal(s) : FID1B.CH
Acq On : 20 Aug 2021 21:53
Operator : DD\AJ
Sample : M3467-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
SAMPLE-10-(410.75)

Integration File: autoint1.e
Quant Time: Aug 20 22:47:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE081621.M
Quant Title :
QLast Update : Mon Aug 16 16:04:52 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.660	7570031	25.768 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082021\
Data File : FE034199.D
Signal(s) : FID1B.CH
Acq On : 20 Aug 2021 21:53
Operator : DD\AJ
Sample : M3467-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
SAMPLE-10-(410.75)

Integration File: autoint1.e
Quant Time: Aug 20 22:47:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE081621.M
Quant Title :
QLast Update : Mon Aug 16 16:04:52 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

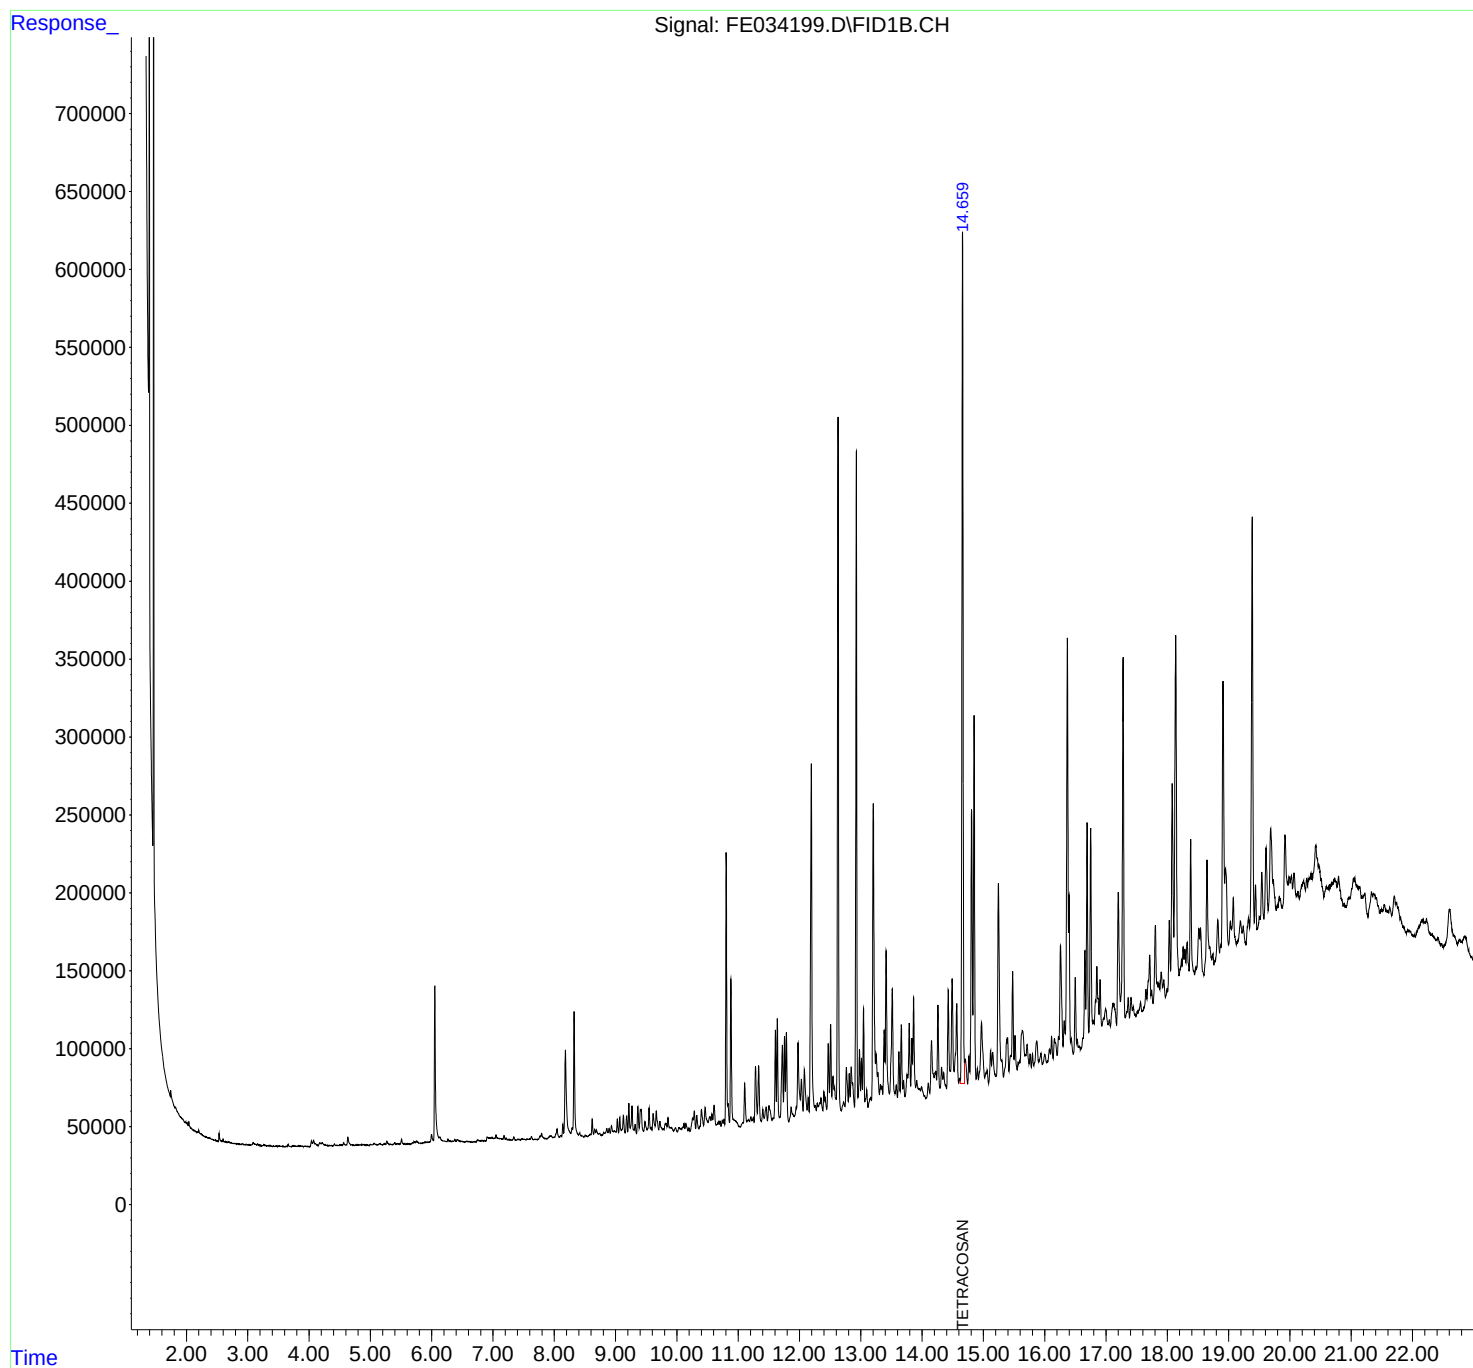

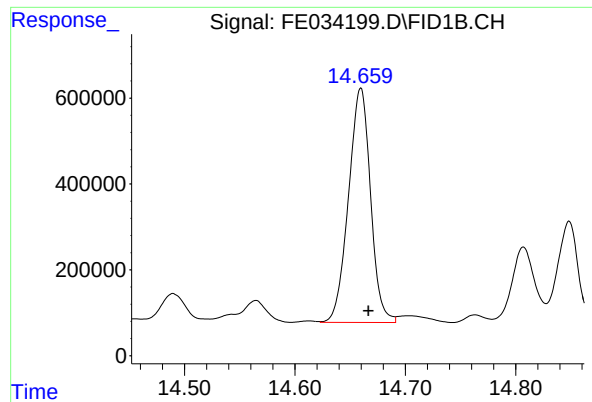

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.660 min
Delta R.T.: -0.007 min
Response: 7570031
Conc: 25.77 ug/ml

Instrument :
FID_E
ClientSampleId :
SAMPLE-10-(410.75)