

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE082321\  
 Data File : FE034220.D  
 Signal(s) : FID1B.CH  
 Acq On : 23 Aug 2021 12:12  
 Operator : DD\AJ  
 Sample : M3467-01 10X  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Aug 24 01:07:23 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE081621.M  
 Quant Title :  
 QLast Update : Mon Aug 16 16:04:52 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.    | Response | Conc Units  |
|-------------------------------|---------|----------|-------------|
| -----                         |         |          |             |
| System Monitoring Compounds   |         |          |             |
| 9) S TETRACOSANE-d50 (SURR... | 14.652  | 817840   | 2.784 ug/ml |
| Target Compounds              |         |          |             |
| 7) N-EICOSANE                 | 12.625f | 764537   | 2.157 ug/ml |
| 10) N-TETRACOSANE             | 14.843  | 686209   | 1.988 ug/ml |
| 15) N-TETRATRIACONTANE        | 19.392f | 145466   | 0.580 ug/ml |
| -----                         |         |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE082321\  
Data File : FE034220.D  
Signal(s) : FID1B.CH  
Acq On : 23 Aug 2021 12:12  
Operator : DD\AJ  
Sample : M3467-01 10X  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Aug 24 01:07:23 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE081621.M  
Quant Title :  
QLast Update : Mon Aug 16 16:04:52 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

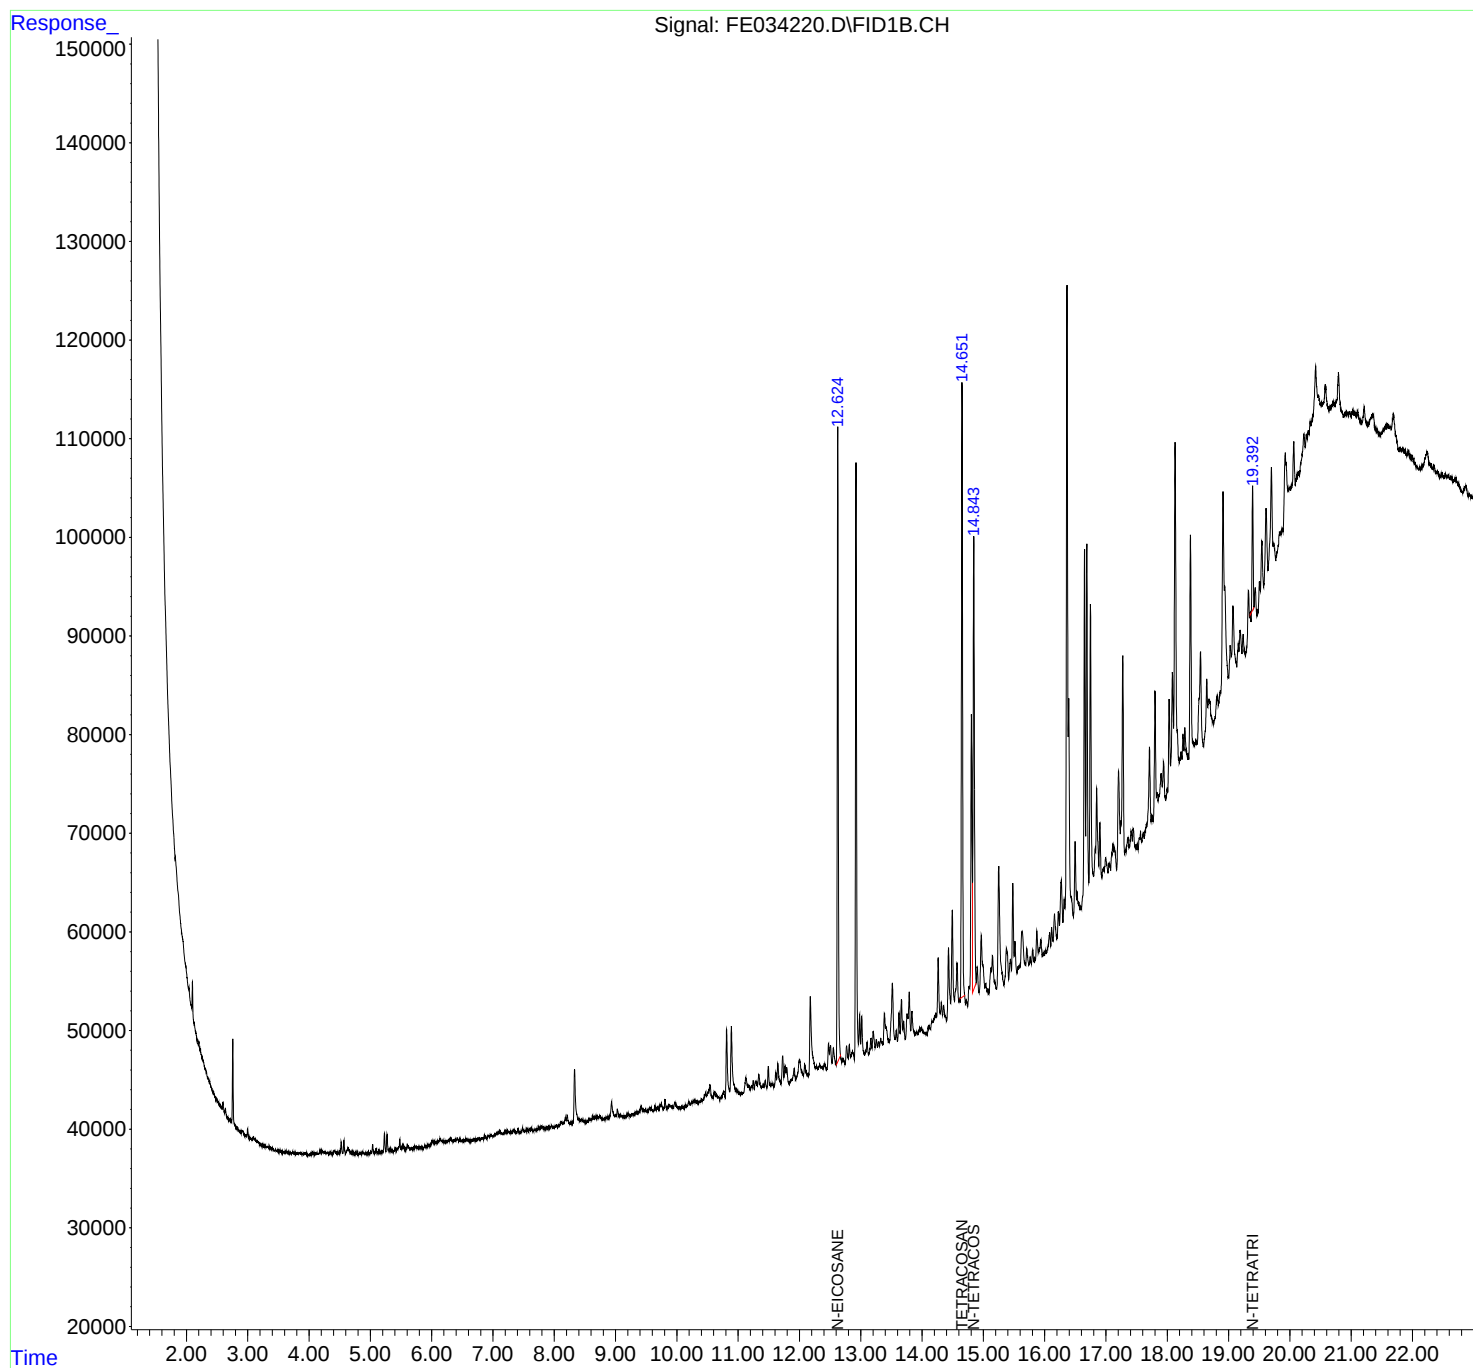


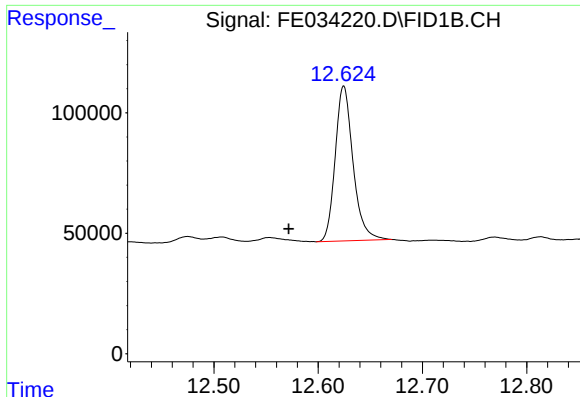

#7 N-EICOSANE


R.T.: 12.625 min  
Delta R.T.: 0.053 min  
Response: 764537  
Conc: 2.16 ug/ml

Instrument :  
FID\_E  
ClientSampleId :

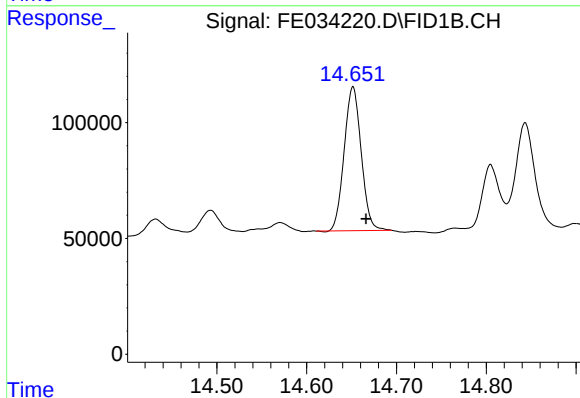


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.652 min  
Delta R.T.: -0.015 min  
Response: 817840  
Conc: 2.78 ug/ml

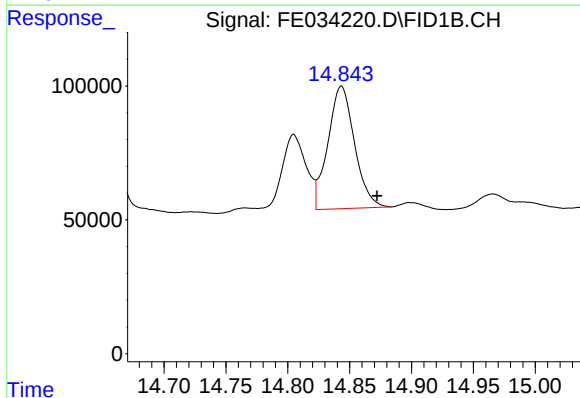

#10 N-TETRACOSANE

R.T.: 14.843 min  
Delta R.T.: -0.029 min  
Response: 686209  
Conc: 1.99 ug/ml

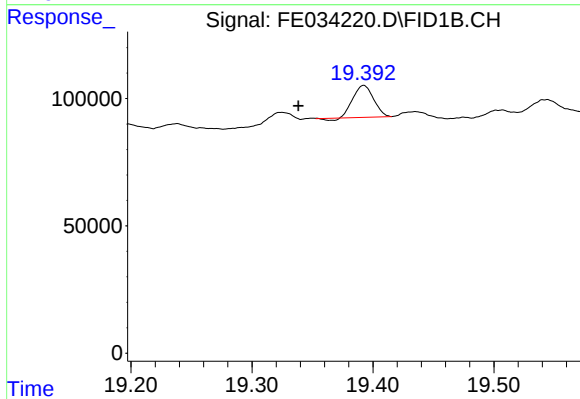

#15 N-TETRATRIACONTANE

R.T.: 19.392 min  
Delta R.T.: 0.054 min  
Response: 145466  
Conc: 0.58 ug/ml