

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082324AL\
 Data File : FE049719.D
 Signal(s) : FID1B.ch
 Acq On : 23 Aug 2024 07:41
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 24 01:15:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 081424.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 14 11:05:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

10) T	n-Eicosane (C20)	12.859	169143	1.133 ug/ml
11) T	n-Heneicosane (C21)	13.477	206604	1.408 ug/ml
13) T	n-Docosane (C22)	14.066	42620	0.292 ug/ml
14) T	n-Tetracosane (C24)	15.168	169198	1.163 ug/ml
15) T	n-Hexacosane (C26)	16.189	57839	0.401 ug/ml
16) T	n-Octacosane (C28)	17.137	134959	0.937 ug/ml
17) T	n-Tricontane (C30)	18.024	185415	1.239 ug/ml
18) T	n-Dotriacontane (C32)	18.855	235303	1.555 ug/ml
19) T	n-Tetratriacontane (C34)	19.638	168940	1.105 ug/ml
20) T	n-Hexatriacontane (C36)	20.378	84559	0.557 ug/ml
21) T	n-Octatriacontane (C38)	21.107	45611	0.291 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082324AL\
Data File : FE049719.D
Signal(s) : FID1B.ch
Acq On : 23 Aug 2024 07:41
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 24 01:15:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 081424.M
Quant Title : GC Extractables
QLast Update : Wed Aug 14 11:05:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

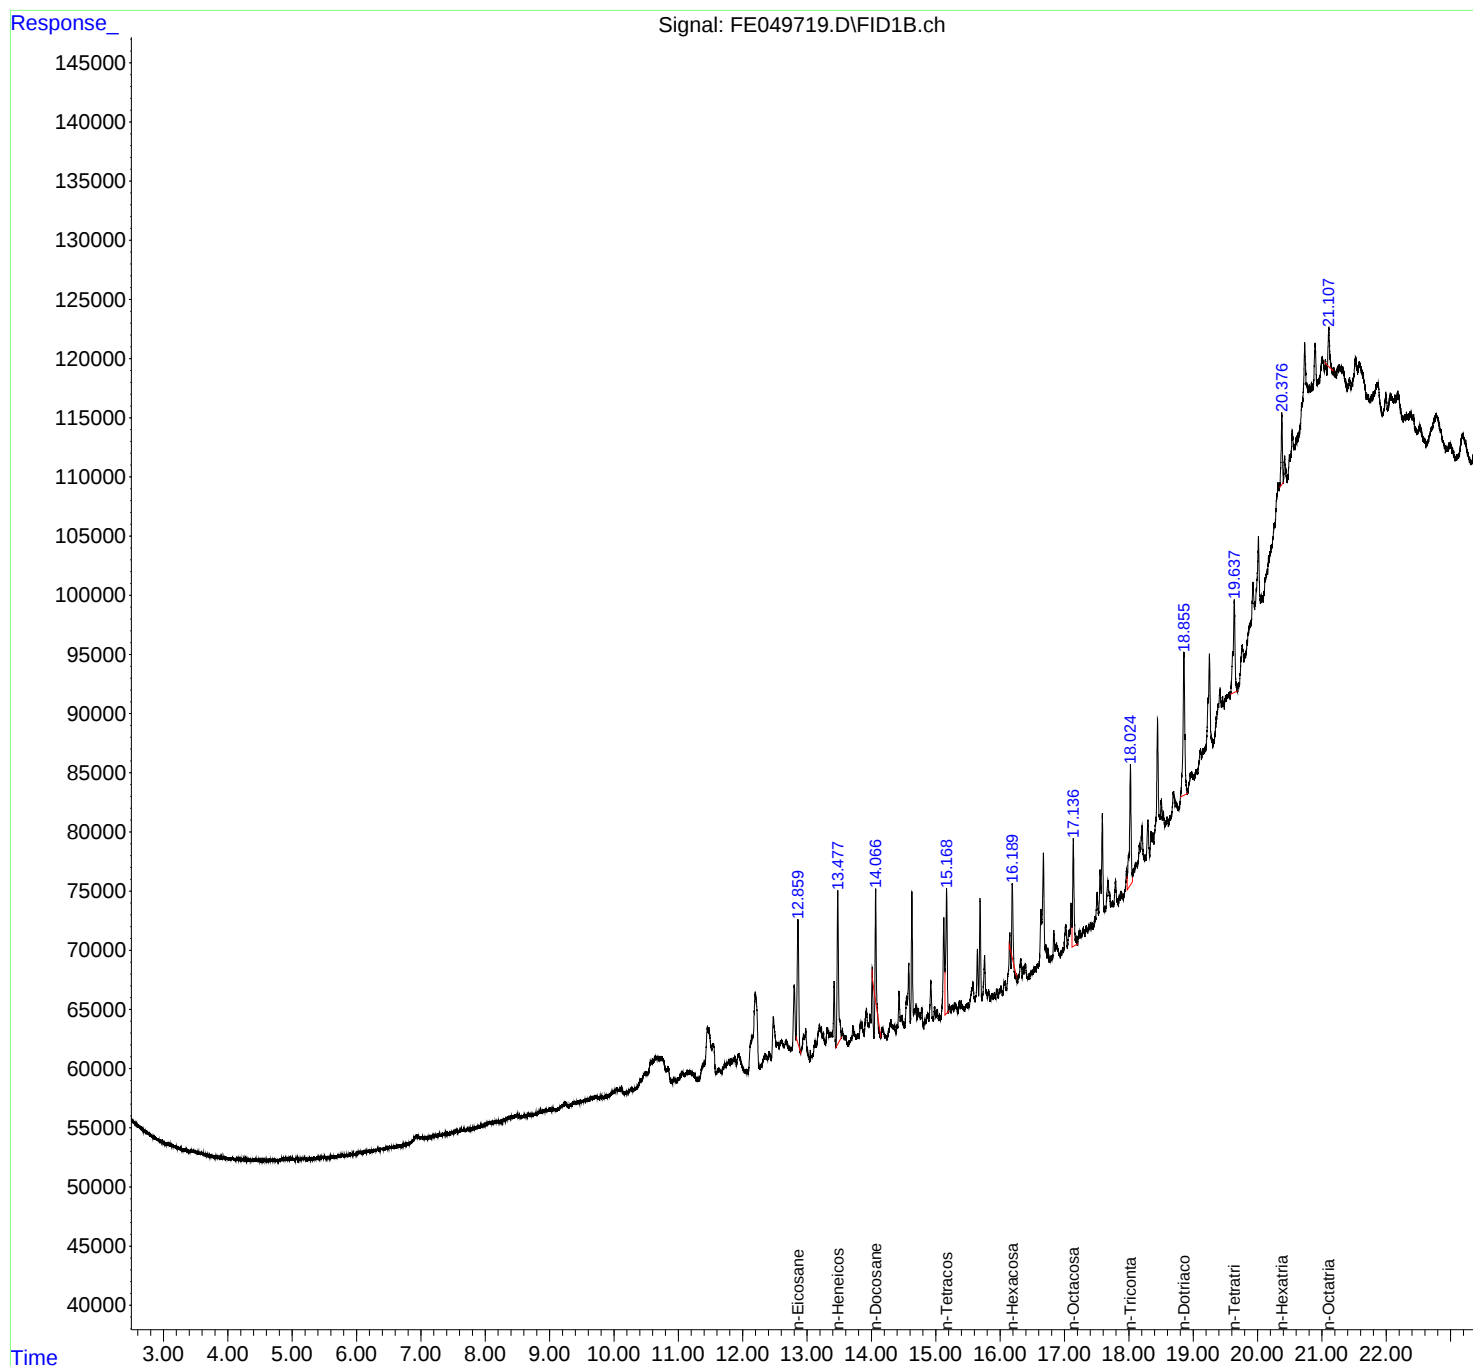


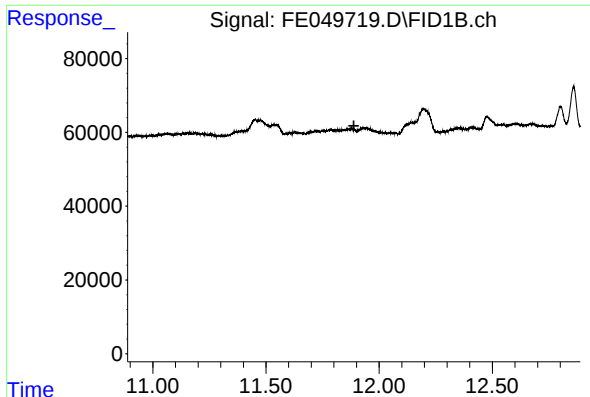

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.888 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

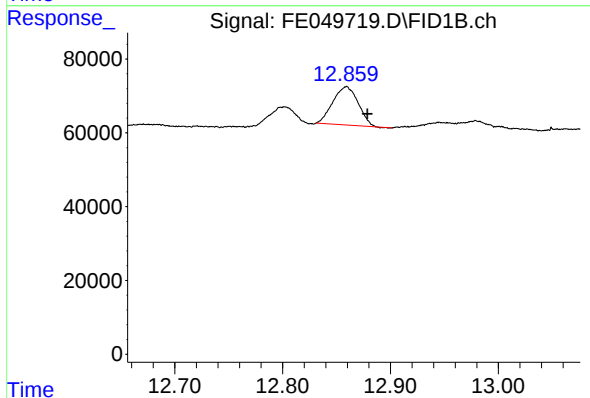


#10 n-Eicosane (C20)

R.T.: 12.859 min
Delta R.T.: -0.020 min
Response: 169143
Conc: 1.13 ug/ml

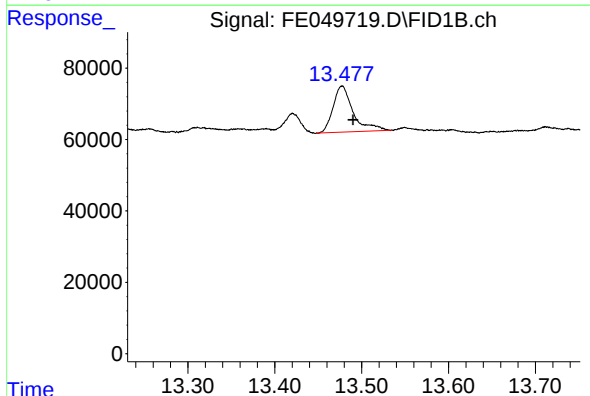


#11 n-Heneicosane (C21)

R.T.: 13.477 min
Delta R.T.: -0.013 min
Response: 206604
Conc: 1.41 ug/ml

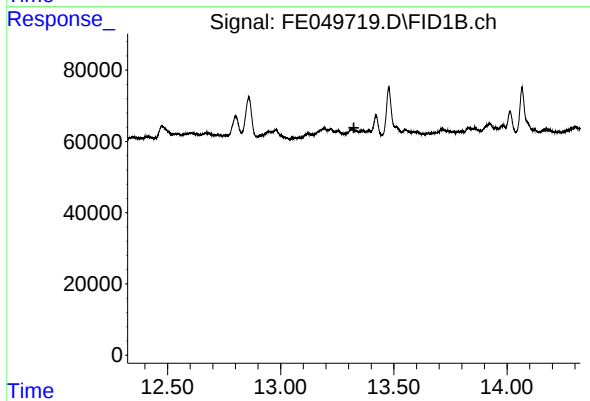

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.323 min
Response: 0
Conc: N.D.

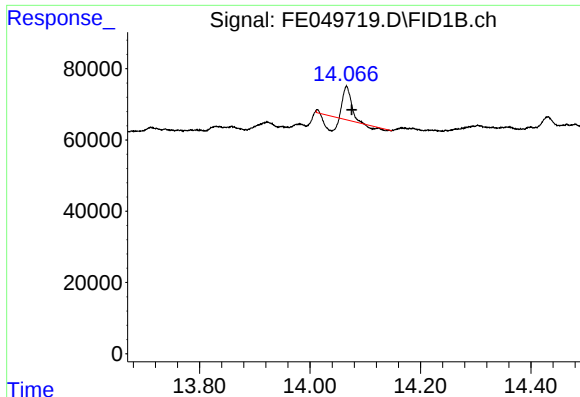

#13 n-Docosane (C22)


R.T.: 14.066 min
Delta R.T.: -0.009 min
Response: 42620
Conc: 0.29 ug/ml

Instrument :
FID_E
ClientSampleId :

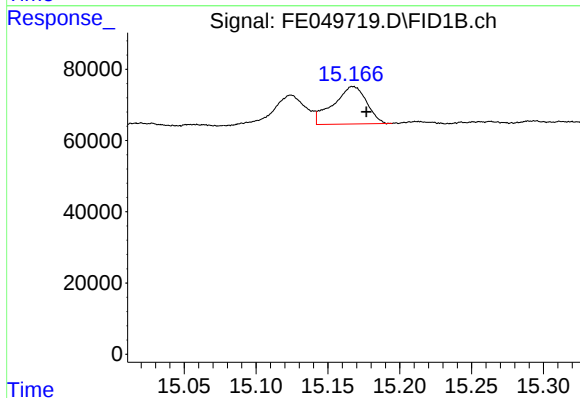


#14 n-Tetracosane (C24)

R.T.: 15.168 min
Delta R.T.: -0.009 min
Response: 169198
Conc: 1.16 ug/ml

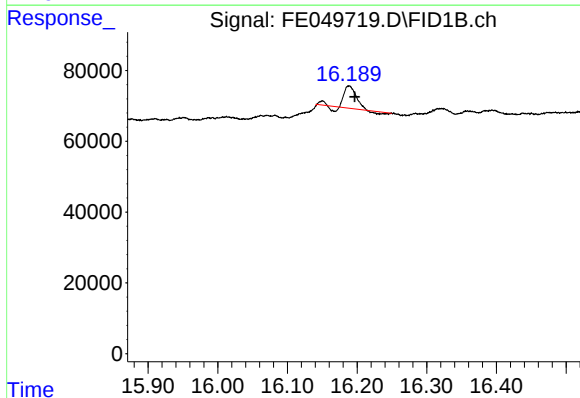


#15 n-Hexacosane (C26)

R.T.: 16.189 min
Delta R.T.: -0.008 min
Response: 57839
Conc: 0.40 ug/ml

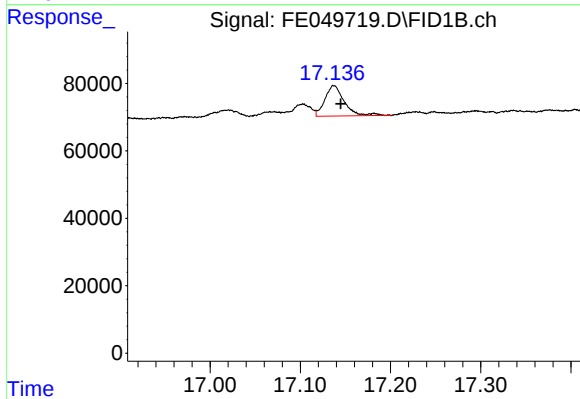

#16 n-Octacosane (C28)


R.T.: 17.137 min
Delta R.T.: -0.008 min
Response: 134959
Conc: 0.94 ug/ml

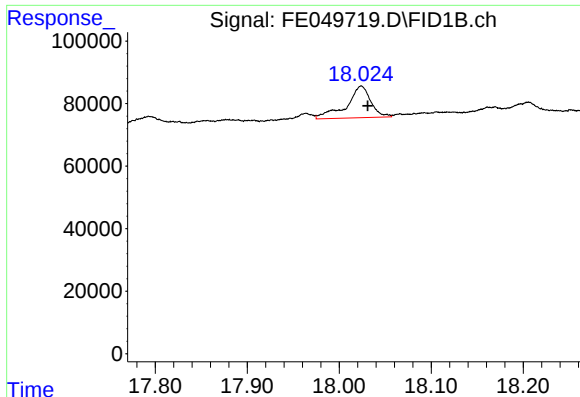

#17 n-Tricontane (C30)


R.T.: 18.024 min
Delta R.T.: -0.007 min
Response: 185415
Conc: 1.24 ug/ml

Instrument :
FID_E
ClientSampleId :

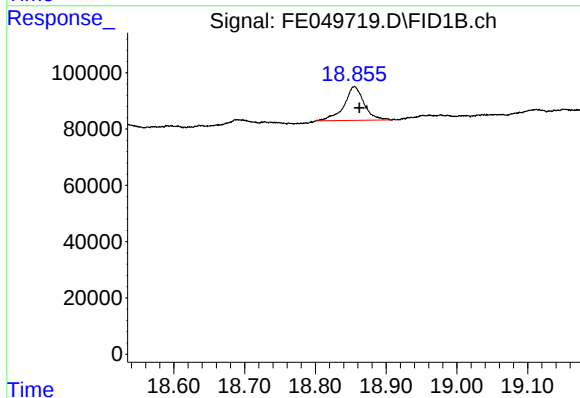


#18 n-Dotriacontane (C32)

R.T.: 18.855 min
Delta R.T.: -0.007 min
Response: 235303
Conc: 1.56 ug/ml

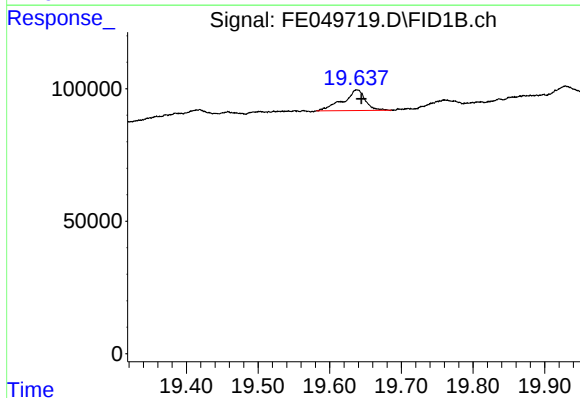


#19 n-Tetratriacontane (C34)

R.T.: 19.638 min
Delta R.T.: -0.006 min
Response: 168940
Conc: 1.11 ug/ml

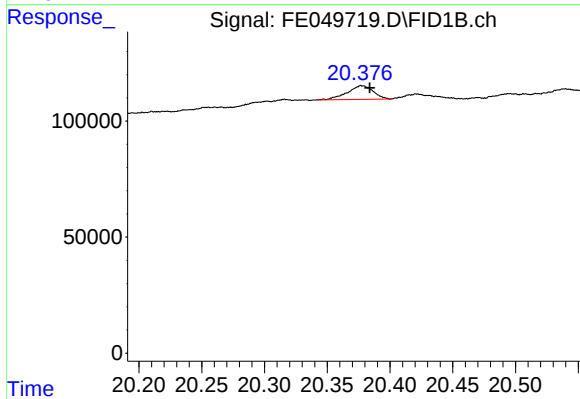

#20 n-Hexatriacontane (C36)

R.T.: 20.378 min
Delta R.T.: -0.006 min
Response: 84559
Conc: 0.56 ug/ml

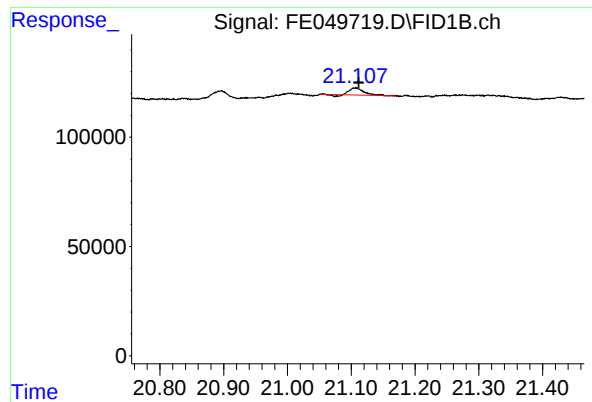

#21 n-Octatriacontane (C38)

R.T.: 21.107 min
Delta R.T.: -0.005 min
Response: 45611
Conc: 0.29 ug/ml

Instrument :

FID_E

ClientSampleId :