

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082421\
Data File : FE034248.D
Signal(s) : FID1B.CH
Acq On : 24 Aug 2021 12:26
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Aug 25 03:58:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE081621.M
Quant Title :
QLast Update : Mon Aug 16 16:04:52 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
10)	N-TETRACOSANE	14.830	238935	0.692 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082421\
Data File : FE034248.D
Signal(s) : FID1B.CH
Acq On : 24 Aug 2021 12:26
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Aug 25 03:58:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE081621.M
Quant Title :
QLast Update : Mon Aug 16 16:04:52 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

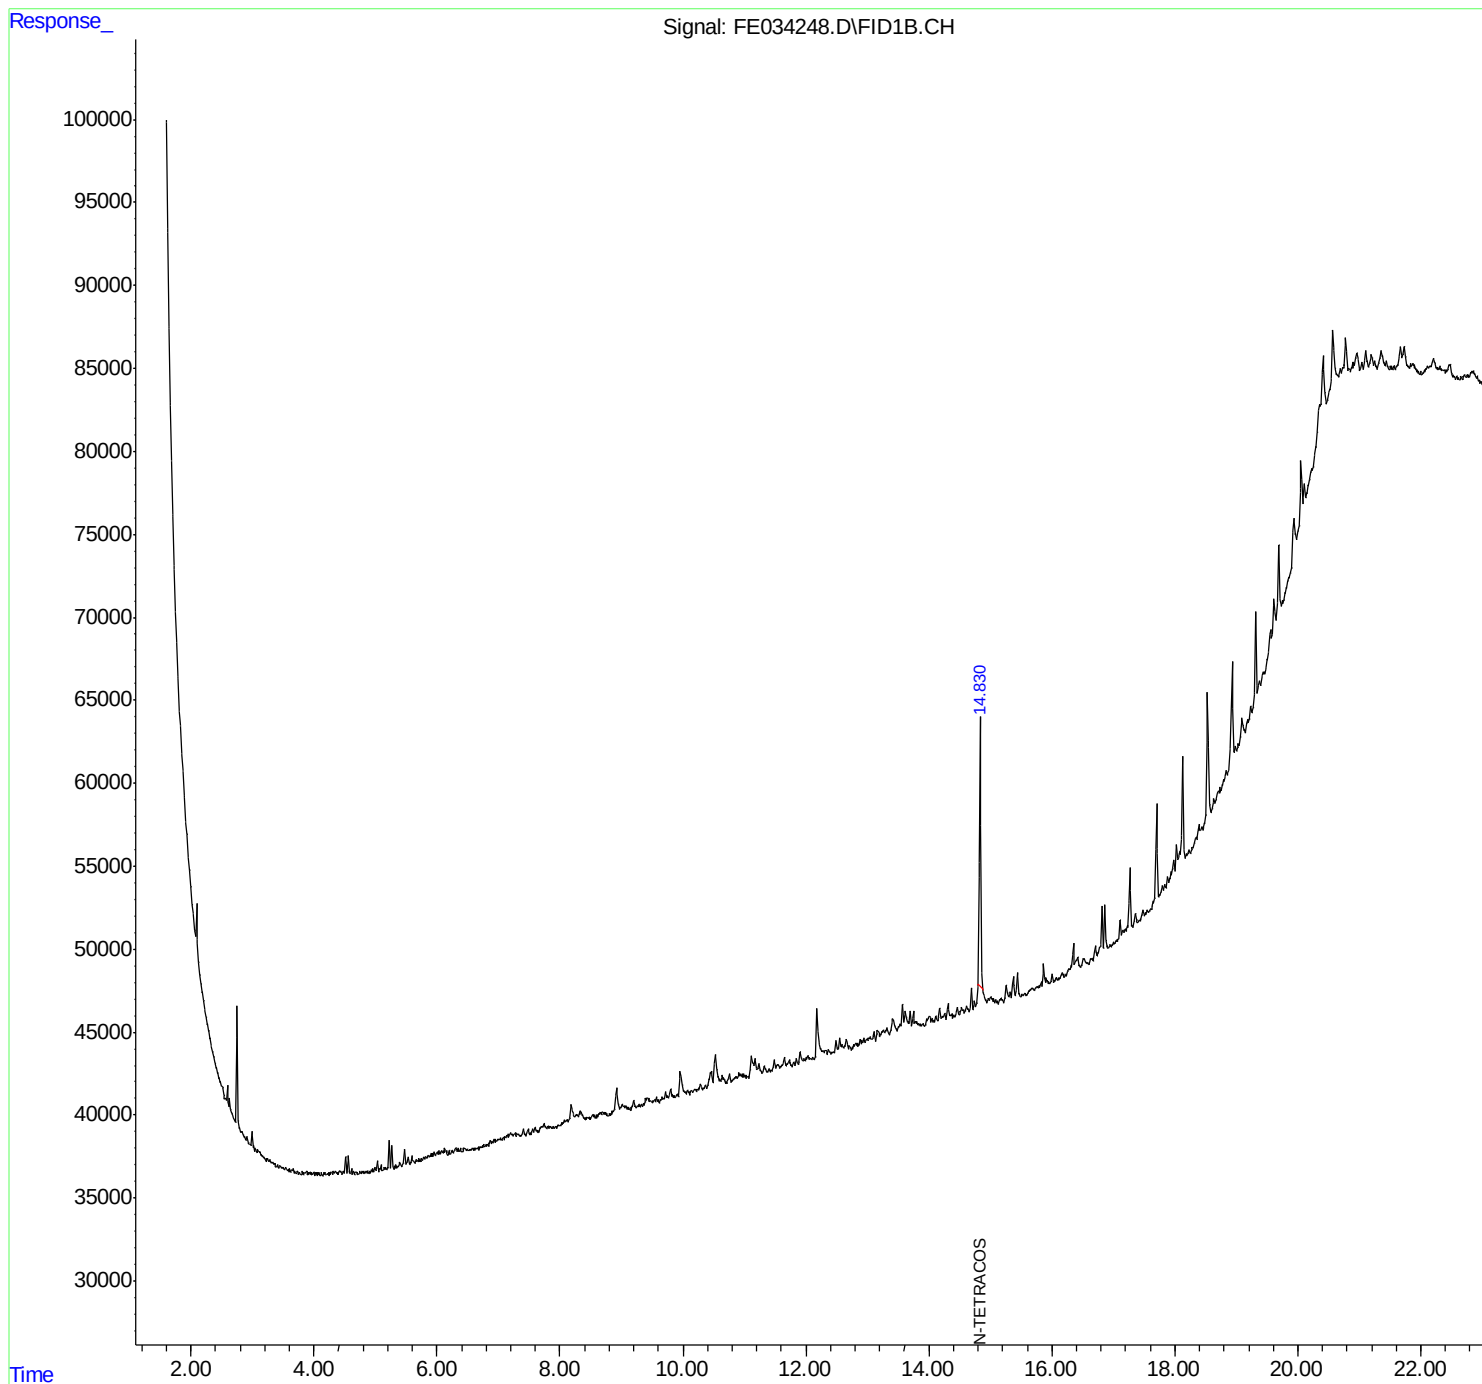


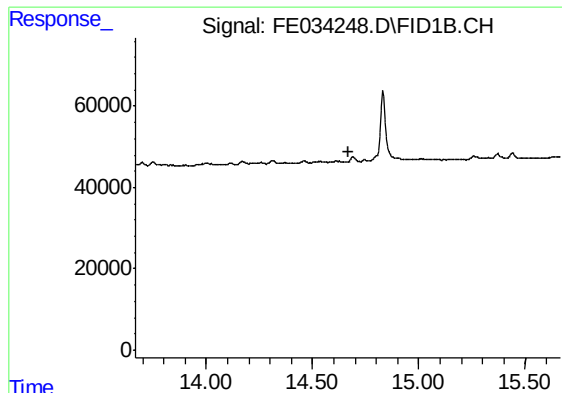

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.666 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
MECL2

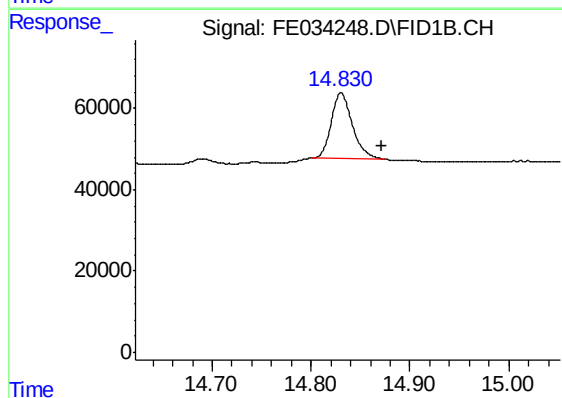

#10 N-TETRACOSANE

R.T.: 14.830 min
Delta R.T.: -0.042 min
Response: 238935
Conc: 0.69 ug/ml