

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082421\
Data File : FE034256.D
Signal(s) : FID1B.CH
Acq On : 24 Aug 2021 17:38
Operator : DD\AJ
Sample : M3505-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
DRILL-CUTTING

Integration File: Sample.e
Quant Time: Aug 25 04:00:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE081621.M
Quant Title :
QLast Update : Mon Aug 16 16:04:52 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.645	4844339	16.490 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082421\
Data File : FE034256.D
Signal(s) : FID1B.CH
Acq On : 24 Aug 2021 17:38
Operator : DD\AJ
Sample : M3505-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
DRILL-CUTTING

Integration File: Sample.e
Quant Time: Aug 25 04:00:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE081621.M
Quant Title :
QLast Update : Mon Aug 16 16:04:52 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

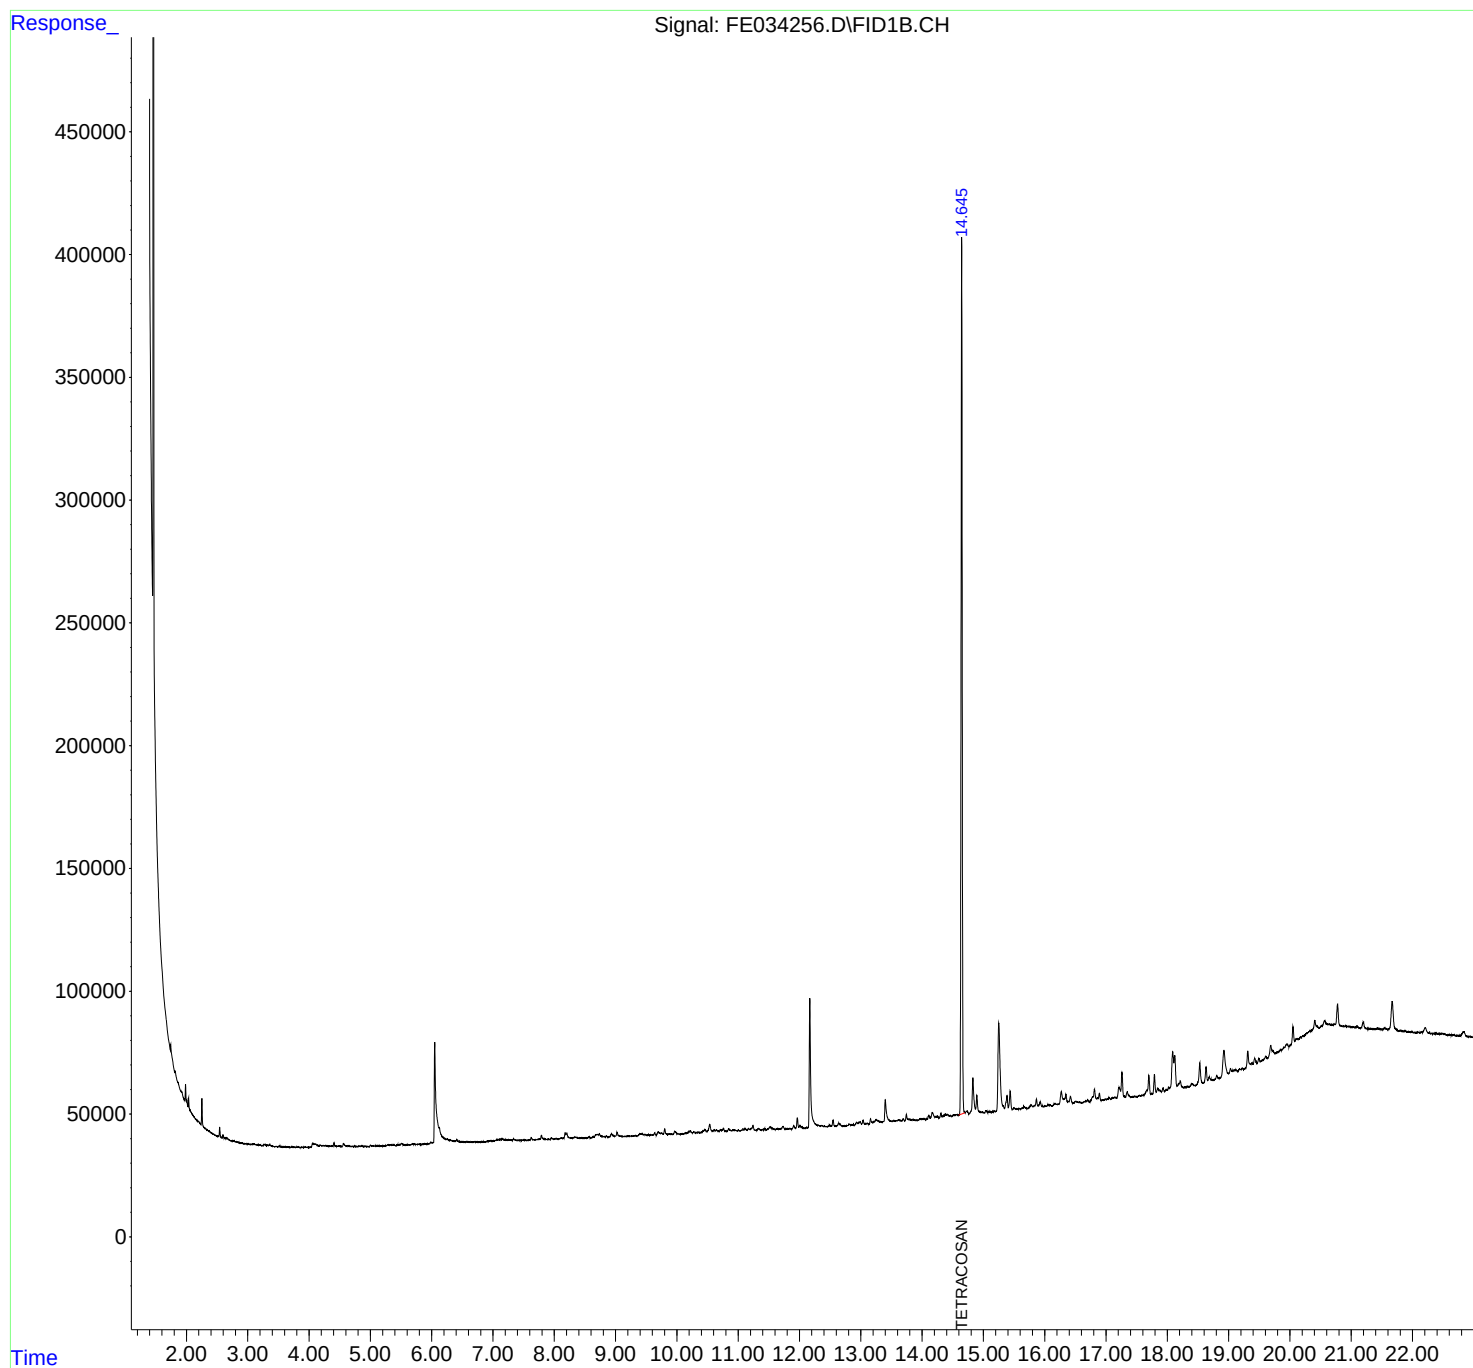

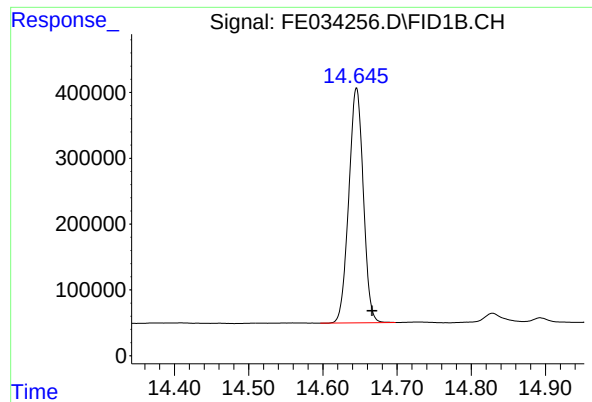

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.645 min
Delta R.T.: -0.021 min
Response: 4844339
Conc: 16.49 ug/ml

Instrument :
FID_E
ClientSampleId :
DRILL-CUTTING