

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082422AL\
 Data File : FE037240.D
 Signal(s) : FID1B.ch
 Acq On : 25 Aug 2022 00:40
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 25 02:01:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082322.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 25 01:38:38 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
18) T n-Dotriacontane (C32)	18.620	44091	0.296 ug/ml
20) T n-Hexatriacontane (C36)	20.167	126368	0.984 ug/ml
21) T n-Octatriacontane (C38)	20.832	262280	2.185 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082422AL\
Data File : FE037240.D
Signal(s) : FID1B.ch
Acq On : 25 Aug 2022 00:40
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 25 02:01:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082322.M
Quant Title : GC Extractables
QLast Update : Thu Aug 25 01:38:38 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

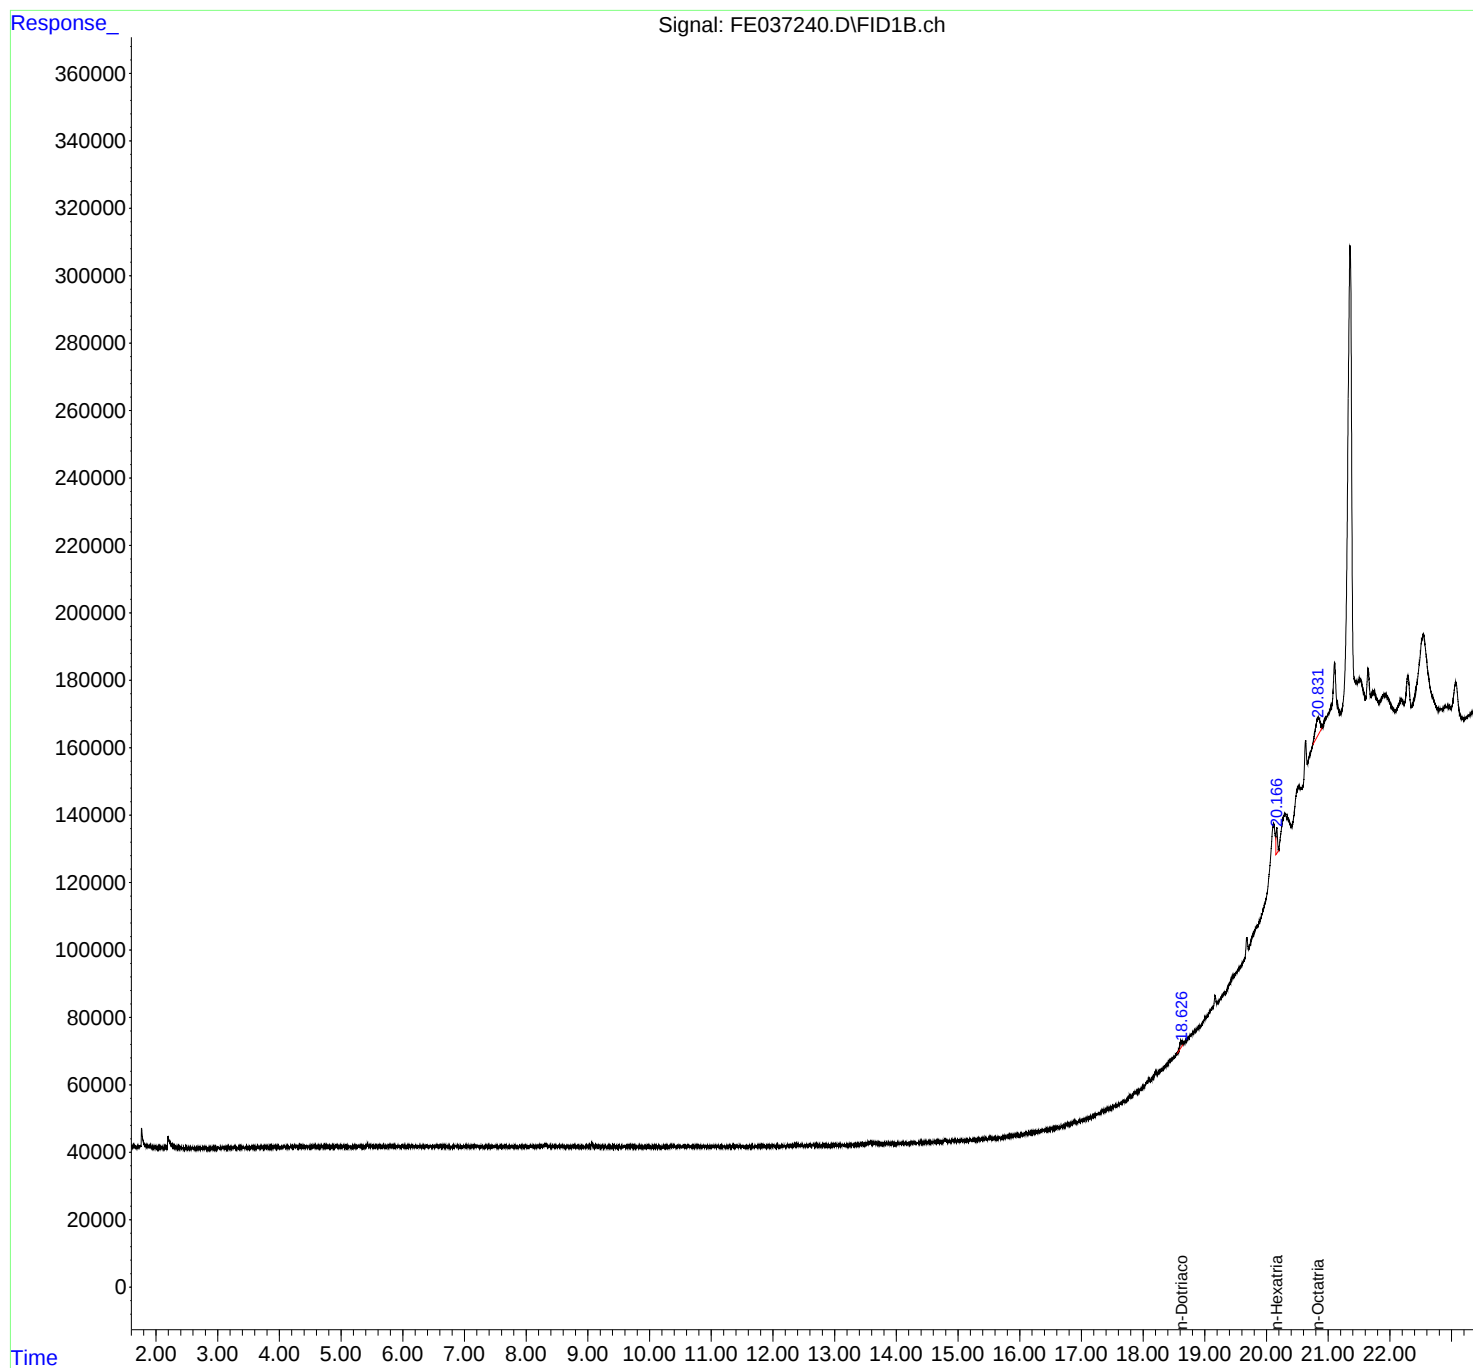


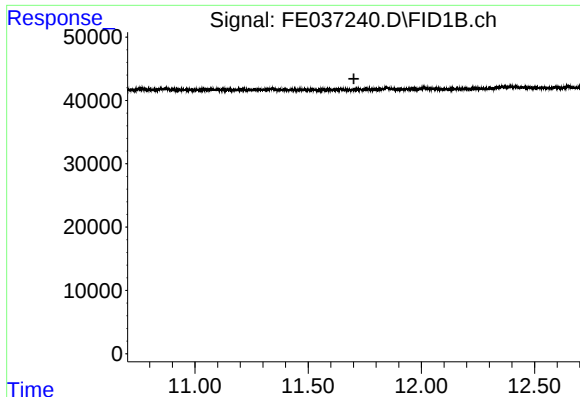

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.702 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

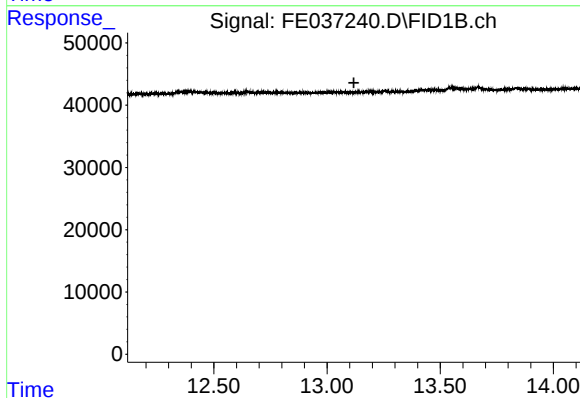


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.119 min
Response: 0
Conc: N.D.

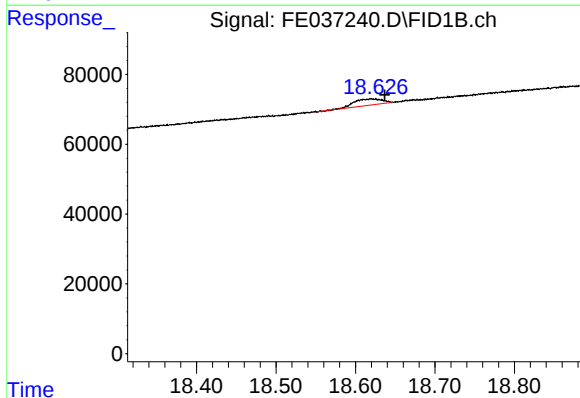


#18 n-Dotriacontane (C32)

R.T.: 18.620 min
Delta R.T.: -0.017 min
Response: 44091
Conc: 0.30 ug/ml

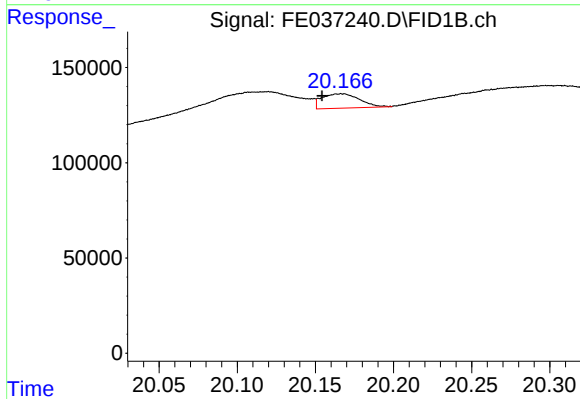

#20 n-Hexatriacontane (C36)

R.T.: 20.167 min
Delta R.T.: 0.013 min
Response: 126368
Conc: 0.98 ug/ml

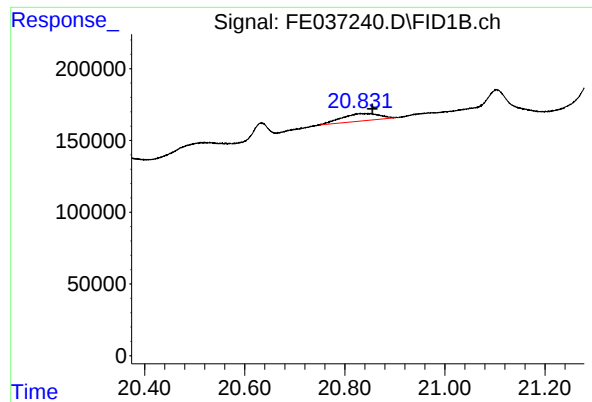

#21 n-Octatriacontane (C38)

R.T.: 20.832 min
Delta R.T.: -0.023 min
Response: 262280
Conc: 2.18 ug/ml

Instrument :

FID_E

ClientSampleId :