

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082522AL\
 Data File : FE037260.D
 Signal(s) : FID1B.ch
 Acq On : 25 Aug 2022 17:20
 Operator : YP\AJ
 Sample : N4352-02D
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 26 03:42:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082322.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 25 01:38:38 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.664	5774671	33.414 ug/ml
Spiked Amount 50.000		Recovery =	66.83%
12) S 1-chlorooctadecane (S...	13.086	4422445	32.368 ug/ml
Spiked Amount 50.000		Recovery =	64.74%
Target Compounds			
10) T n-Eicosane (C20)	12.735f	109852	0.667 ug/ml
14) T n-Tetracosane (C24)	14.927	16547	0.100 ug/ml
16) T n-Octacosane (C28)	16.942	44406	0.280 ug/ml
17) T n-Tricontane (C30)	17.864f	156827	1.010 ug/ml
18) T n-Dotriacontane (C32)	18.655	44761	0.300 ug/ml
19) T n-Tetratriacontane (C34)	19.440	86505	0.644 ug/ml
20) T n-Hexatriacontane (C36)	20.118	22923	0.179 ug/ml
21) T n-Octatriacontane (C38)	20.820	4624	0.039 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082522AL\
Data File : FE037260.D
Signal(s) : FID1B.ch
Acq On : 25 Aug 2022 17:20
Operator : YP\AJ
Sample : N4352-02D
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 26 03:42:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082322.M
Quant Title : GC Extractables
QLast Update : Thu Aug 25 01:38:38 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

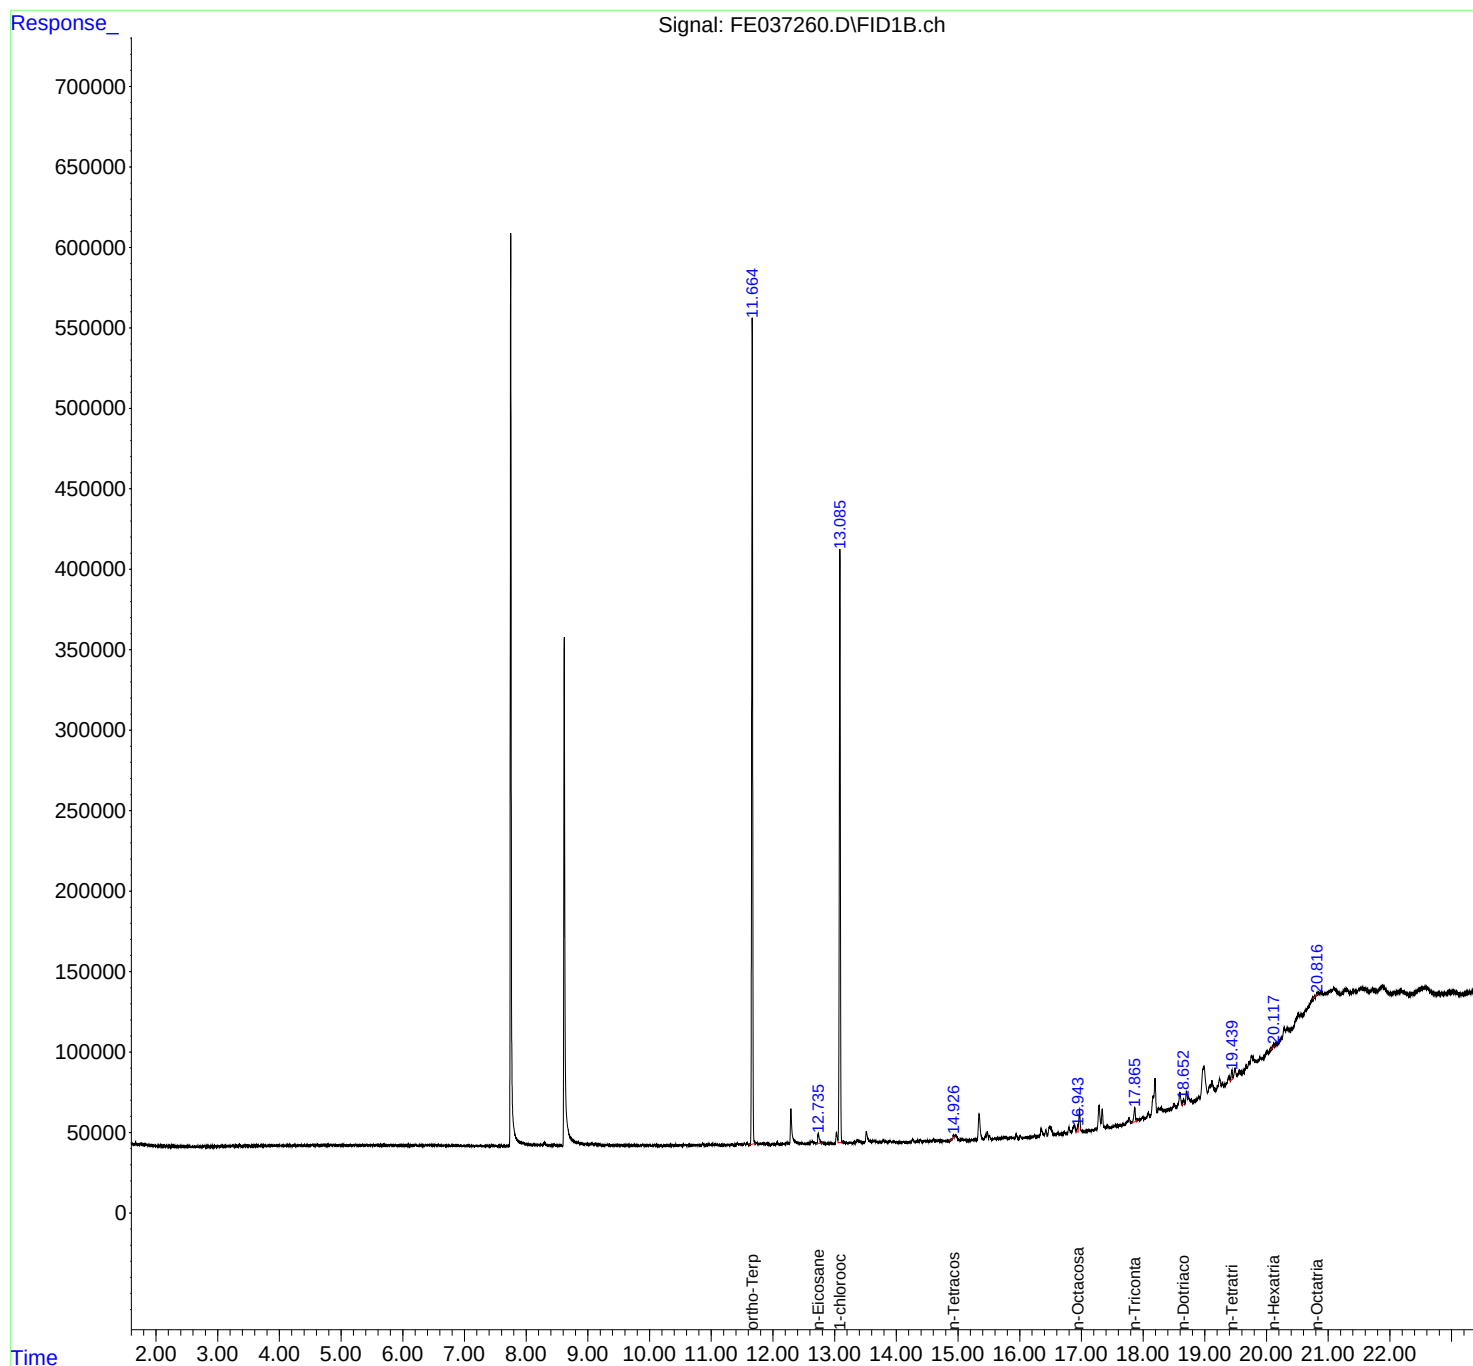


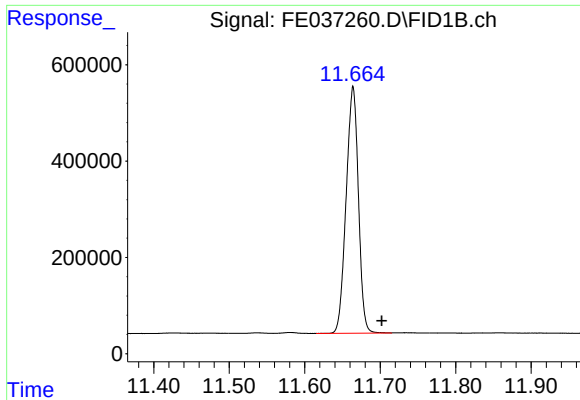

#9 ortho-Terphenyl (SURR)


R.T.: 11.664 min
Delta R.T.: -0.038 min
Response: 5774671
Conc: 33.41 ug/ml

Instrument :
FID_E
ClientSampleId :

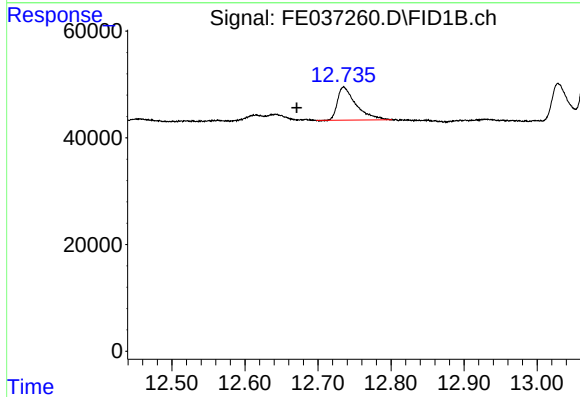


#10 n-Eicosane (C20)

R.T.: 12.735 min
Delta R.T.: 0.064 min
Response: 109852
Conc: 0.67 ug/ml

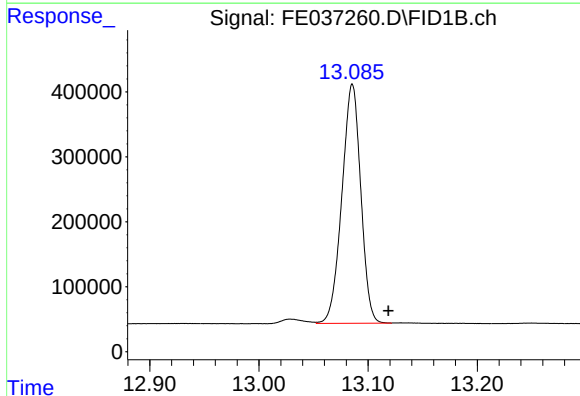


#12 1-chlorooctadecane (SURR)

R.T.: 13.086 min
Delta R.T.: -0.033 min
Response: 4422445
Conc: 32.37 ug/ml

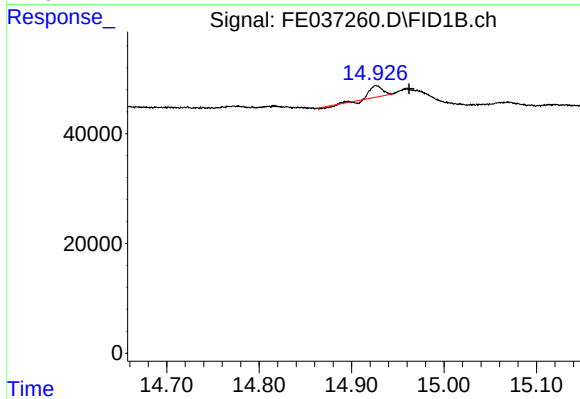

#14 n-Tetracosane (C24)


R.T.: 14.927 min
Delta R.T.: -0.036 min
Response: 16547
Conc: 0.10 ug/ml

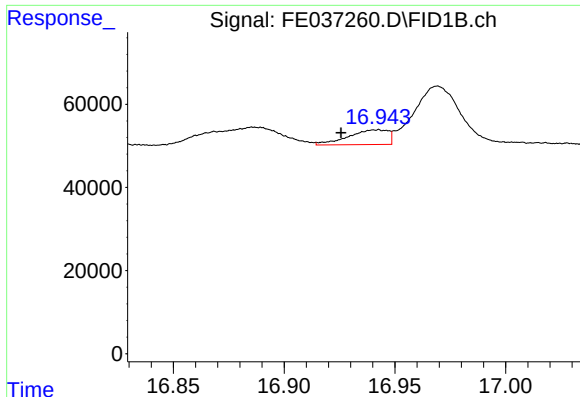

#16 n-Octacosane (C28)


R.T.: 16.942 min
Delta R.T.: 0.016 min
Response: 44406
Conc: 0.28 ug/ml

Instrument :
FID_E
ClientSampleId :

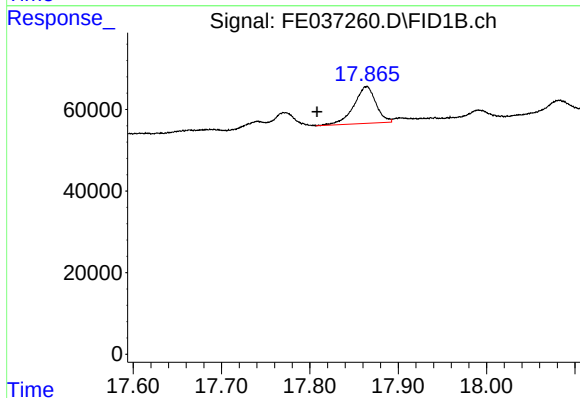


#17 n-Tricontane (C30)

R.T.: 17.864 min
Delta R.T.: 0.056 min
Response: 156827
Conc: 1.01 ug/ml

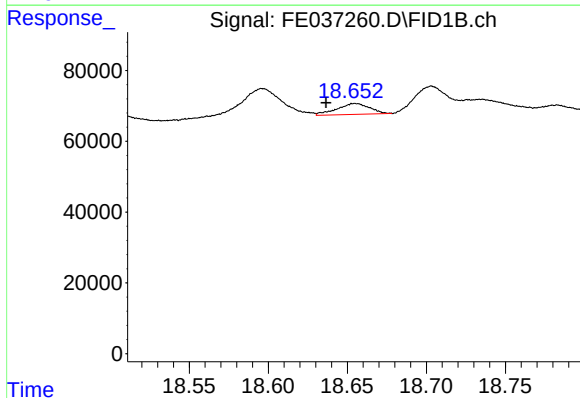


#18 n-Dotriacontane (C32)

R.T.: 18.655 min
Delta R.T.: 0.019 min
Response: 44761
Conc: 0.30 ug/ml

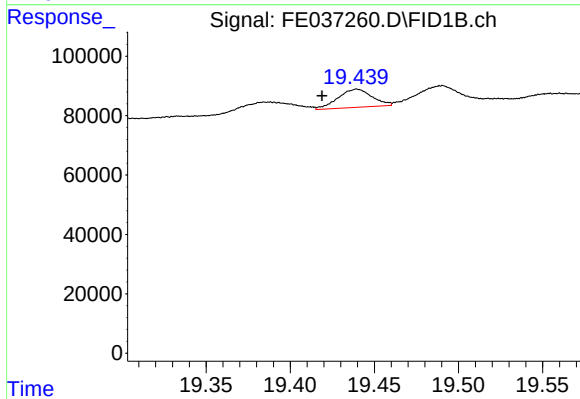

#19 n-Tetratriacontane (C34)


R.T.: 19.440 min
Delta R.T.: 0.021 min
Response: 86505
Conc: 0.64 ug/ml

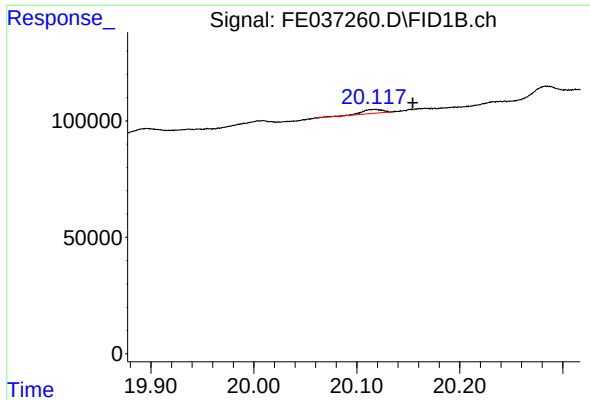

#20 n-Hexatriacontane (C36)

R.T.: 20.118 min
Delta R.T.: -0.036 min
Response: 22923
Conc: 0.18 ug/ml

Instrument :
FID_E
ClientSampleId :

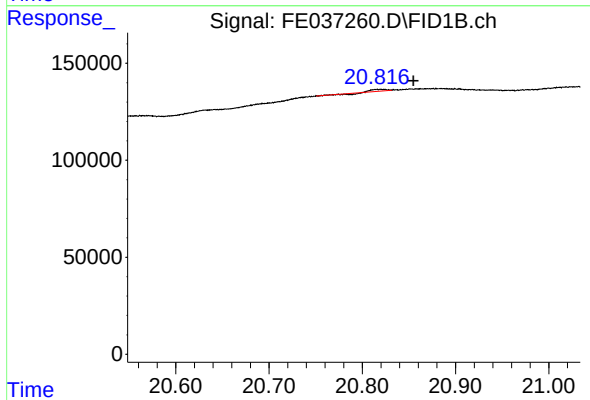

#21 n-Octatriacontane (C38)

R.T.: 20.820 min
Delta R.T.: -0.035 min
Response: 4624
Conc: 0.04 ug/ml