

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC082525AL\
Data File : FC069723.D
Signal(s) : FID1A.ch
Acq On : 25 Aug 2025 13:56
Operator : YP/AJ
Sample : Q2892-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 26 02:10:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 080125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 14:14:17 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.101	3685207	33.802 ug/ml
Spiked Amount 50.000		Recovery =	67.60%
Target Compounds			
6) T n-Tetradecane (C14)	8.292	49975	0.350 ug/ml
18) T n-Dotriacontane (C32)	18.653	56427	0.508 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_C\Data\FC082525AL\
Data File : FC069723.D
Signal(s) : FID1A.ch
Acq On : 25 Aug 2025 13:56
Operator : YP/AJ
Sample : Q2892-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 26 02:10:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_C\Method\Aliphatic EPH 080125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 14:14:17 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

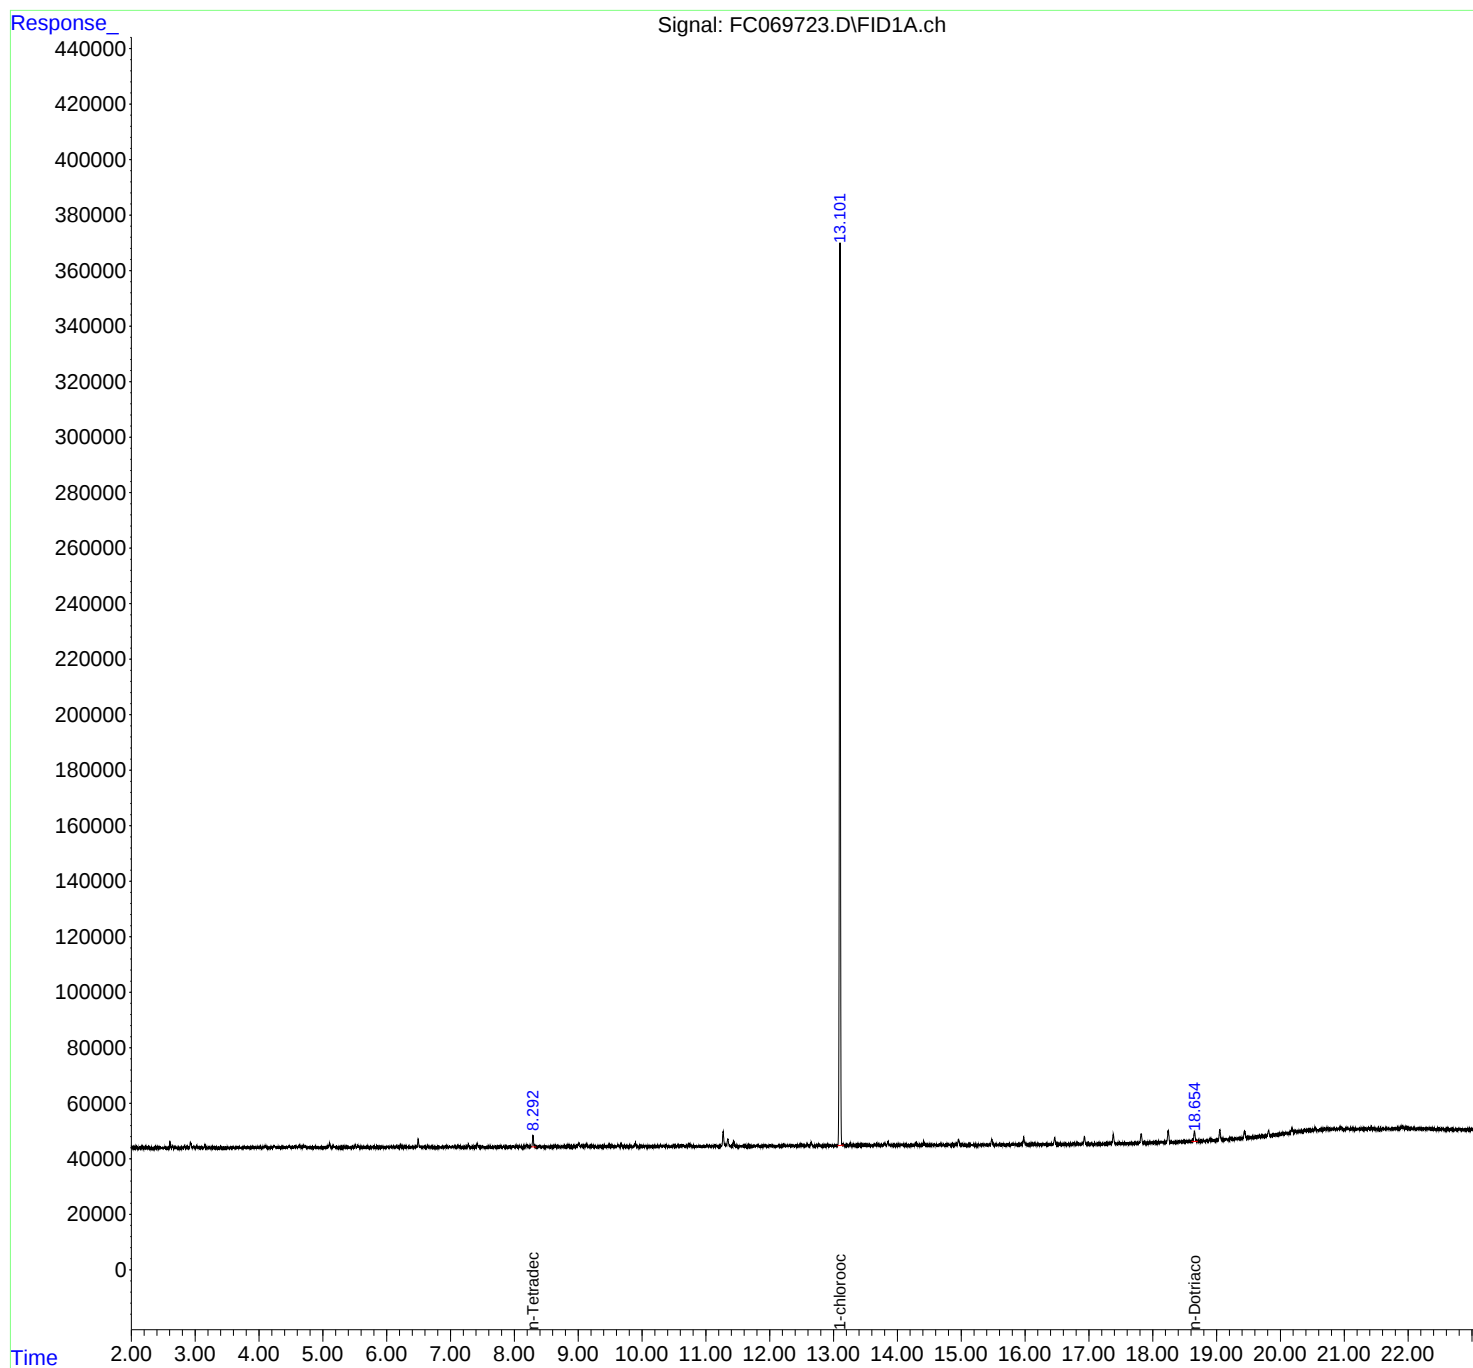


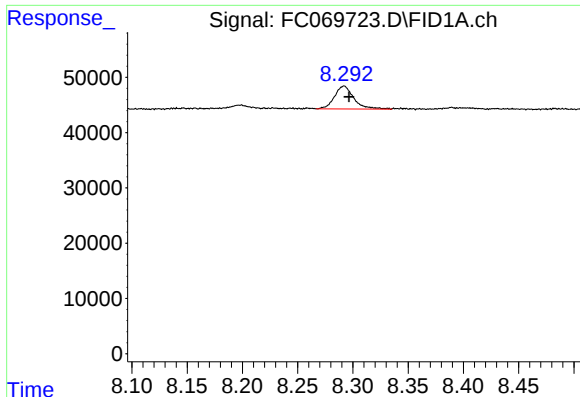

#6 n-Tetradecane (C14)


R.T.: 8.292 min
Delta R.T.: -0.005 min
Response: 49975
Conc: 0.35 ug/ml

Instrument :
FID_E
ClientSampleId :

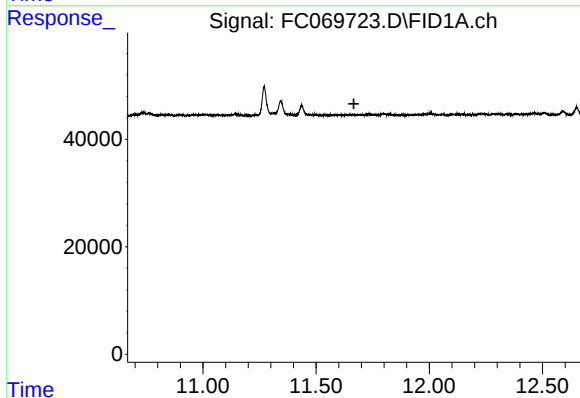


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T. : 11.667 min
Response: 0
Conc: N.D.

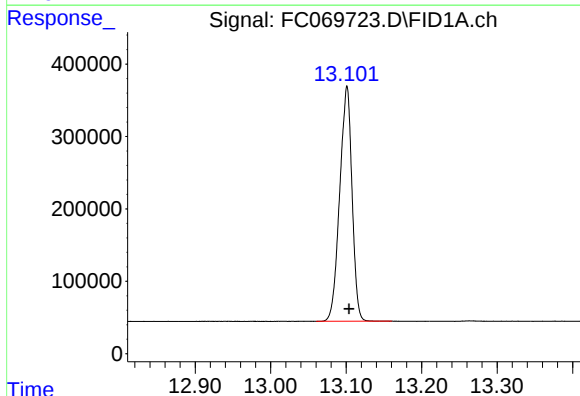

#12 1-chlorooctadecane (SURR)

R.T.: 13.101 min
Delta R.T.: -0.003 min
Response: 3685207
Conc: 33.80 ug/ml

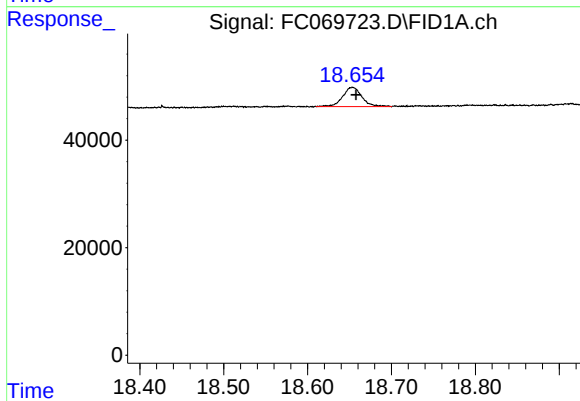

#18 n-Dotriacontane (C32)

R.T.: 18.653 min
Delta R.T.: -0.004 min
Response: 56427
Conc: 0.51 ug/ml