

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082525\
Data File : FF016214.D
Signal(s) : FID2B.ch
Acq On : 25 Aug 2025 23:31
Operator : YP\AJ
Sample : PB169376BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 26 04:27:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080625.M
Quant Title :
QLast Update : Wed Aug 06 13:50:48 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	15.079	2229786	19.976 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.983	48547	0.390 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082525\
Data File : FF016214.D
Signal(s) : FID2B.ch
Acq On : 25 Aug 2025 23:31
Operator : YP\AJ
Sample : PB169376BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 26 04:27:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080625.M
Quant Title :
QLast Update : Wed Aug 06 13:50:48 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

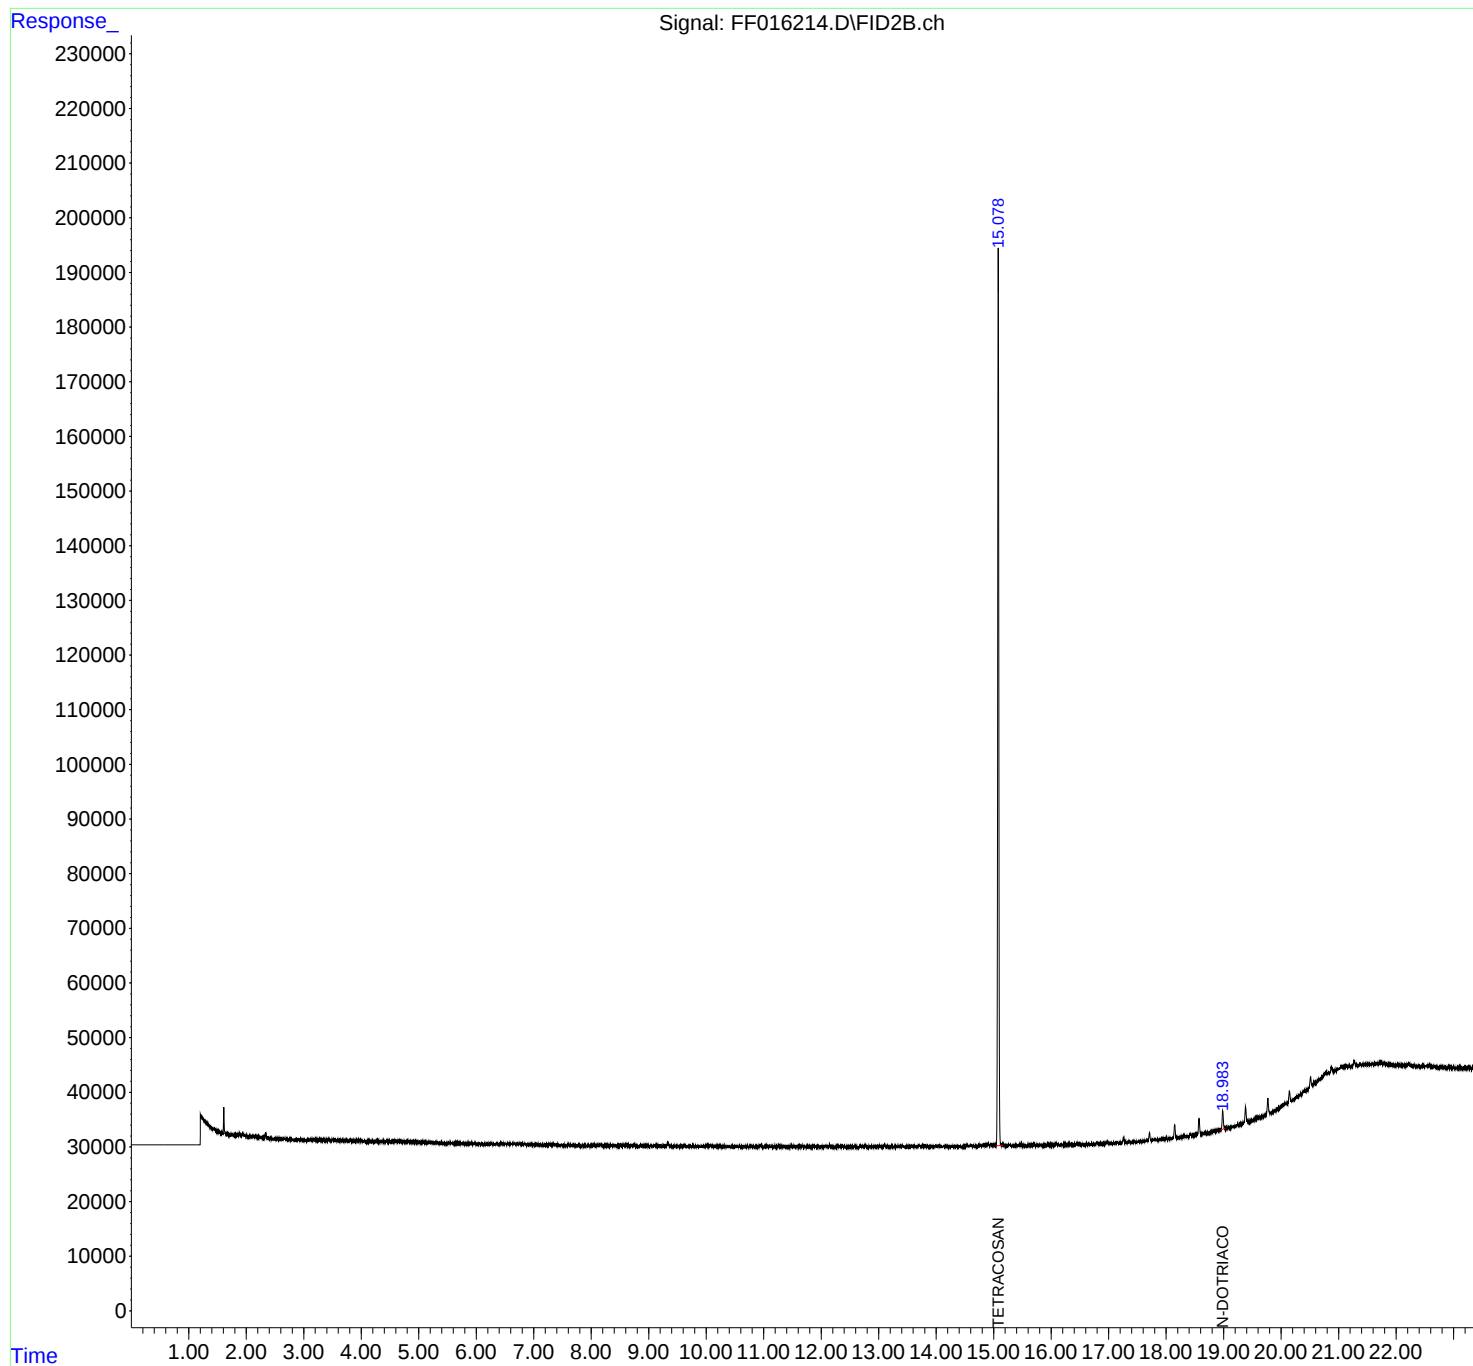


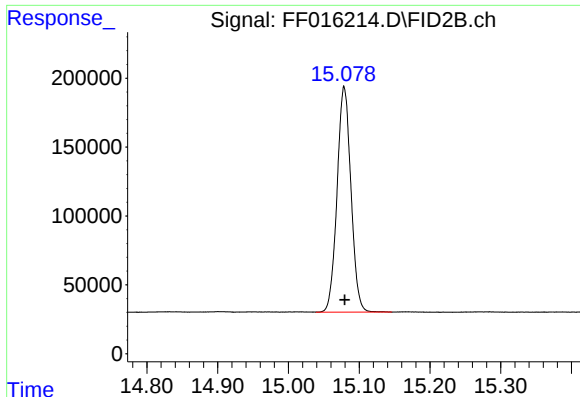

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.079 min
Delta R.T.: 0.000 min
Response: 2229786
Conc: 19.98 ug/ml

Instrument :
FID_E
ClientSampleId :

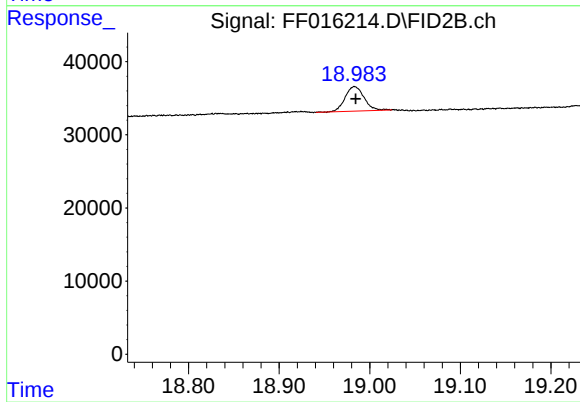

#14 N-DOTRIACONTANE

R.T.: 18.983 min
Delta R.T.: -0.001 min
Response: 48547
Conc: 0.39 ug/ml