

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082622AL\
Data File : FE037271.D
Signal(s) : FID1B.ch
Acq On : 26 Aug 2022 13:24
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 27 02:40:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082322.M
Quant Title : GC Extractables
QLast Update : Sat Aug 27 02:21:03 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
19) T	n-Tetratriacontane (C34)	19.437	365558	2.721 ug/ml
21) T	n-Octatriacontane (C38)	20.910f	37468	0.312 ug/ml
22) T	n-Tetracontane (C40)	21.579f	431760	3.575 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082622AL\
Data File : FE037271.D
Signal(s) : FID1B.ch
Acq On : 26 Aug 2022 13:24
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 27 02:40:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082322.M
Quant Title : GC Extractables
QLast Update : Sat Aug 27 02:21:03 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

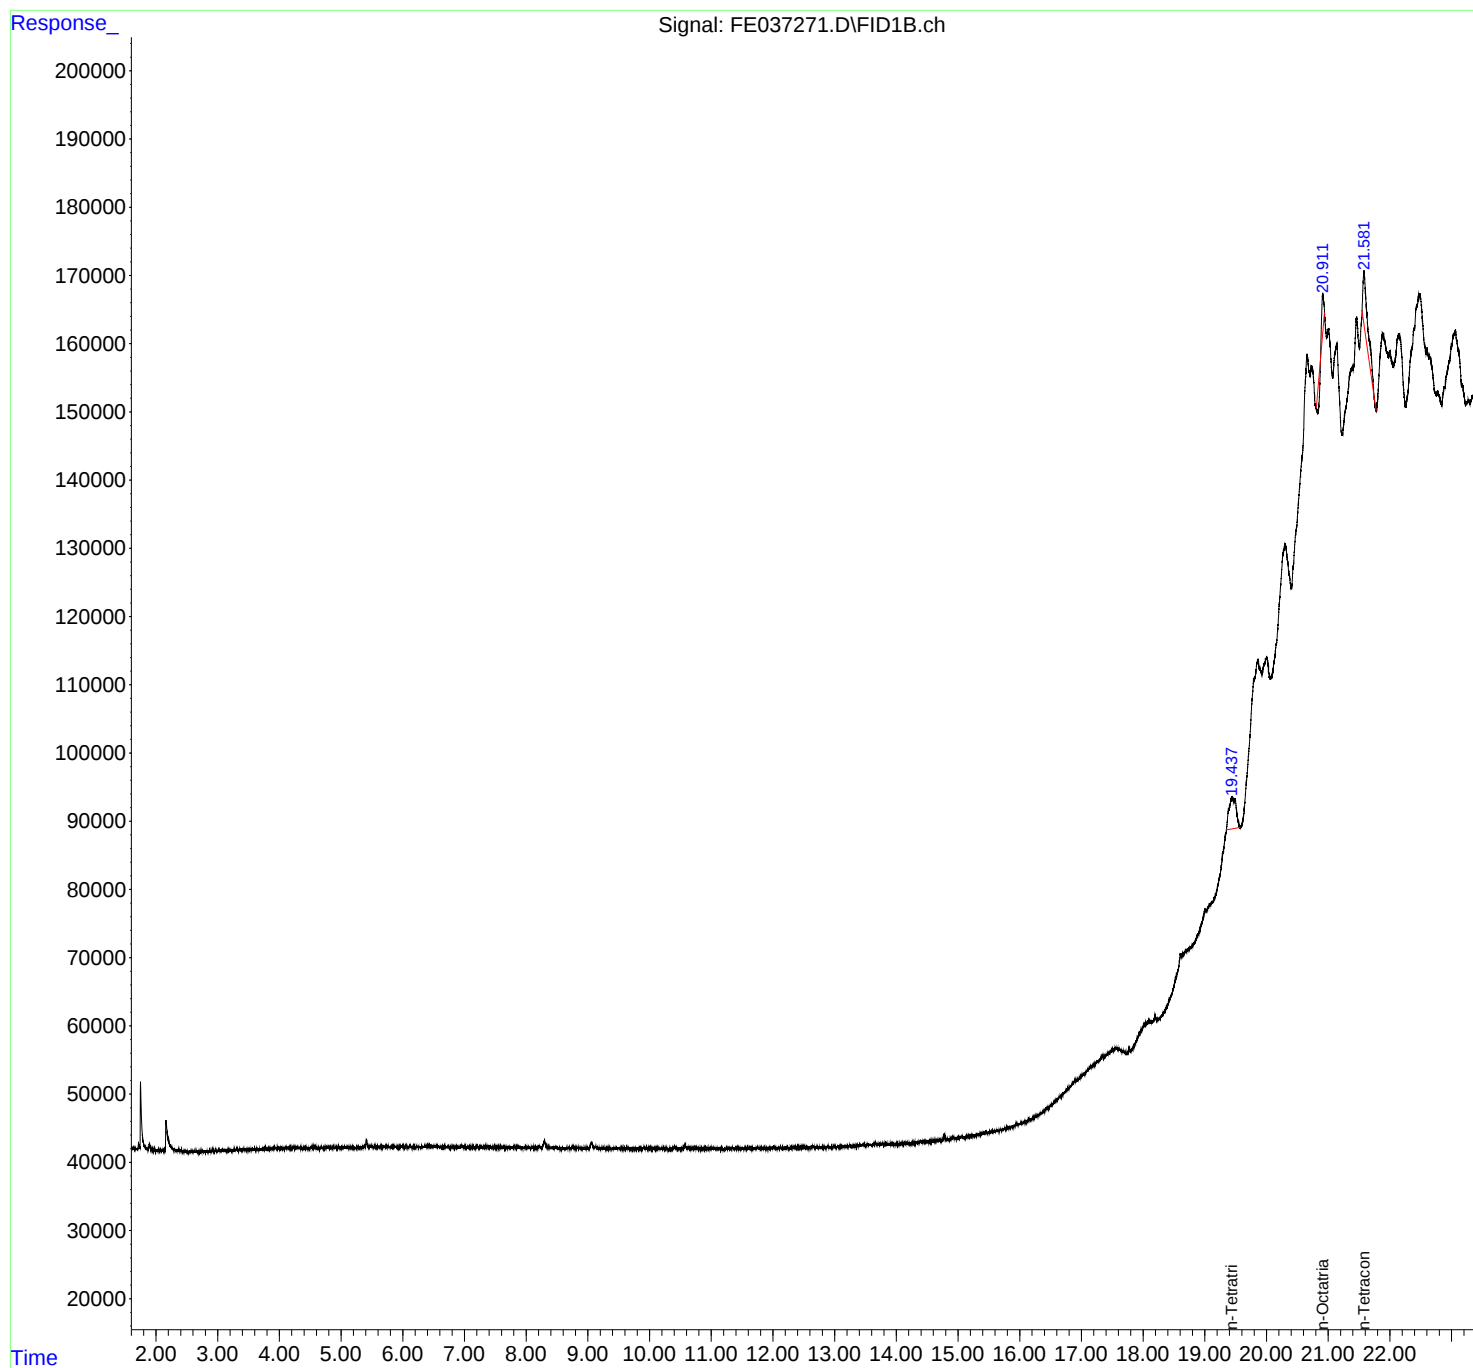


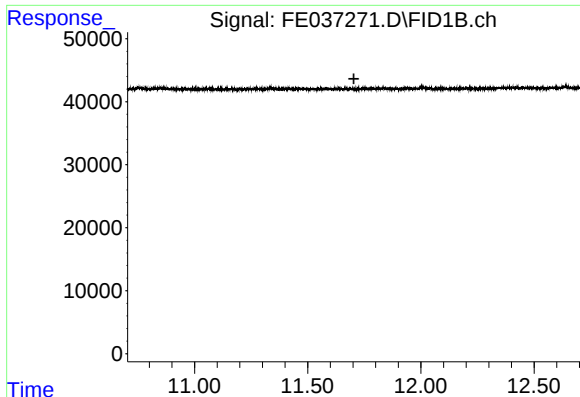

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.704 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

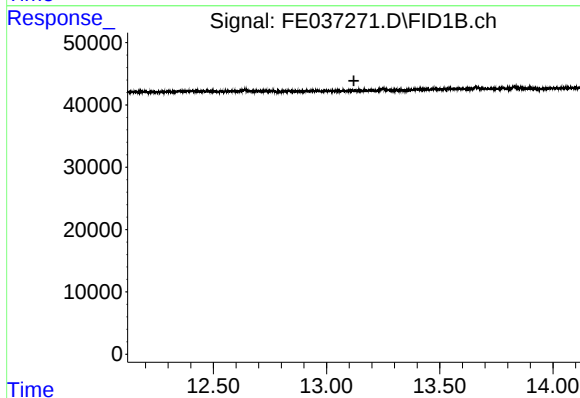


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.121 min
Response: 0
Conc: N.D.

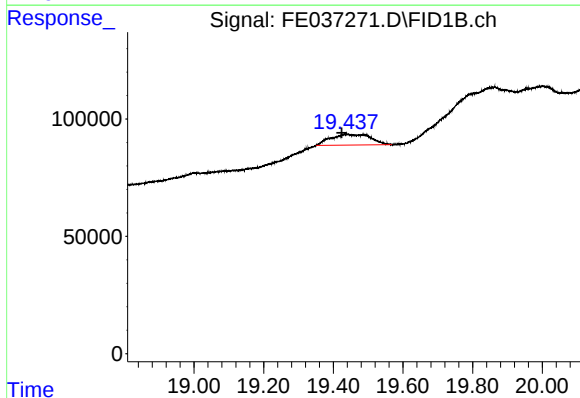


#19 n-Tetratriacontane (C34)

R.T.: 19.437 min
Delta R.T.: 0.013 min
Response: 365558
Conc: 2.72 ug/ml

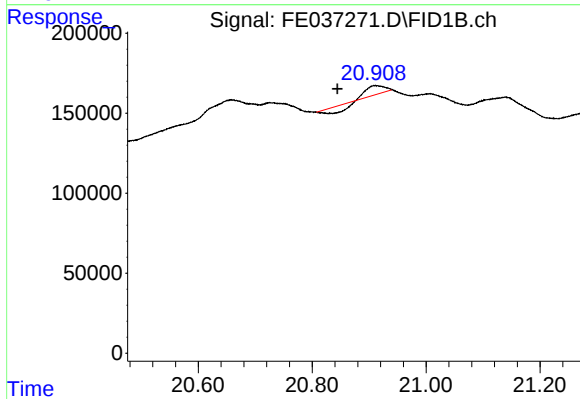

#21 n-Octatriacontane (C38)

R.T.: 20.910 min
Delta R.T.: 0.066 min
Response: 37468
Conc: 0.31 ug/ml

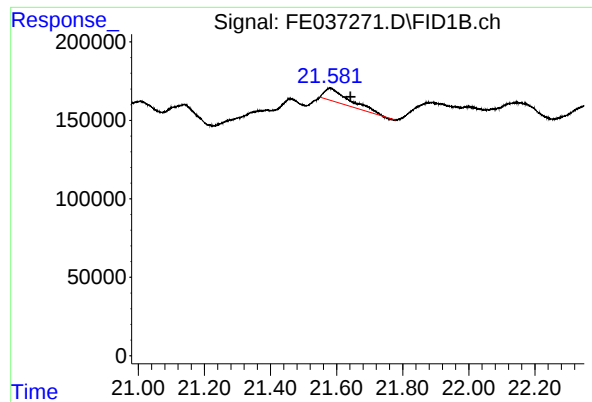

#22 n-Tetracontane (C40)

R.T.: 21.579 min
Delta R.T.: -0.063 min
Response: 431760
Conc: 3.57 ug/ml

Instrument :
FID_E
ClientSampleId :