

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082622AL\
 Data File : FE037276.D
 Signal(s) : FID1B.ch
 Acq On : 26 Aug 2022 17:28
 Operator : YP\AJ
 Sample : N4375-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 27 02:42:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082322.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 27 02:21:03 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.660	5428833	31.413 ug/ml
Spiked Amount 50.000		Recovery =	62.83%
12) S 1-chlorooctadecane (S...	13.081	4216900	30.864 ug/ml
Spiked Amount 50.000		Recovery =	61.73%
Target Compounds			
10) T n-Eicosane (C20)	12.726f	169075	1.027 ug/ml
14) T n-Tetracosane (C24)	14.922	12492	0.076 ug/ml
17) T n-Tricontane (C30)	17.769	51958	0.335 ug/ml
18) T n-Dotriacontane (C32)	18.597	84066	0.564 ug/ml
19) T n-Tetratriacontane (C34)	19.378	55800	0.415 ug/ml
20) T n-Hexatriacontane (C36)	20.114	49431	0.385 ug/ml
21) T n-Octatriacontane (C38)	20.812	36379	0.303 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082622AL\
Data File : FE037276.D
Signal(s) : FID1B.ch
Acq On : 26 Aug 2022 17:28
Operator : YP\AJ
Sample : N4375-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 27 02:42:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082322.M
Quant Title : GC Extractables
QLast Update : Sat Aug 27 02:21:03 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

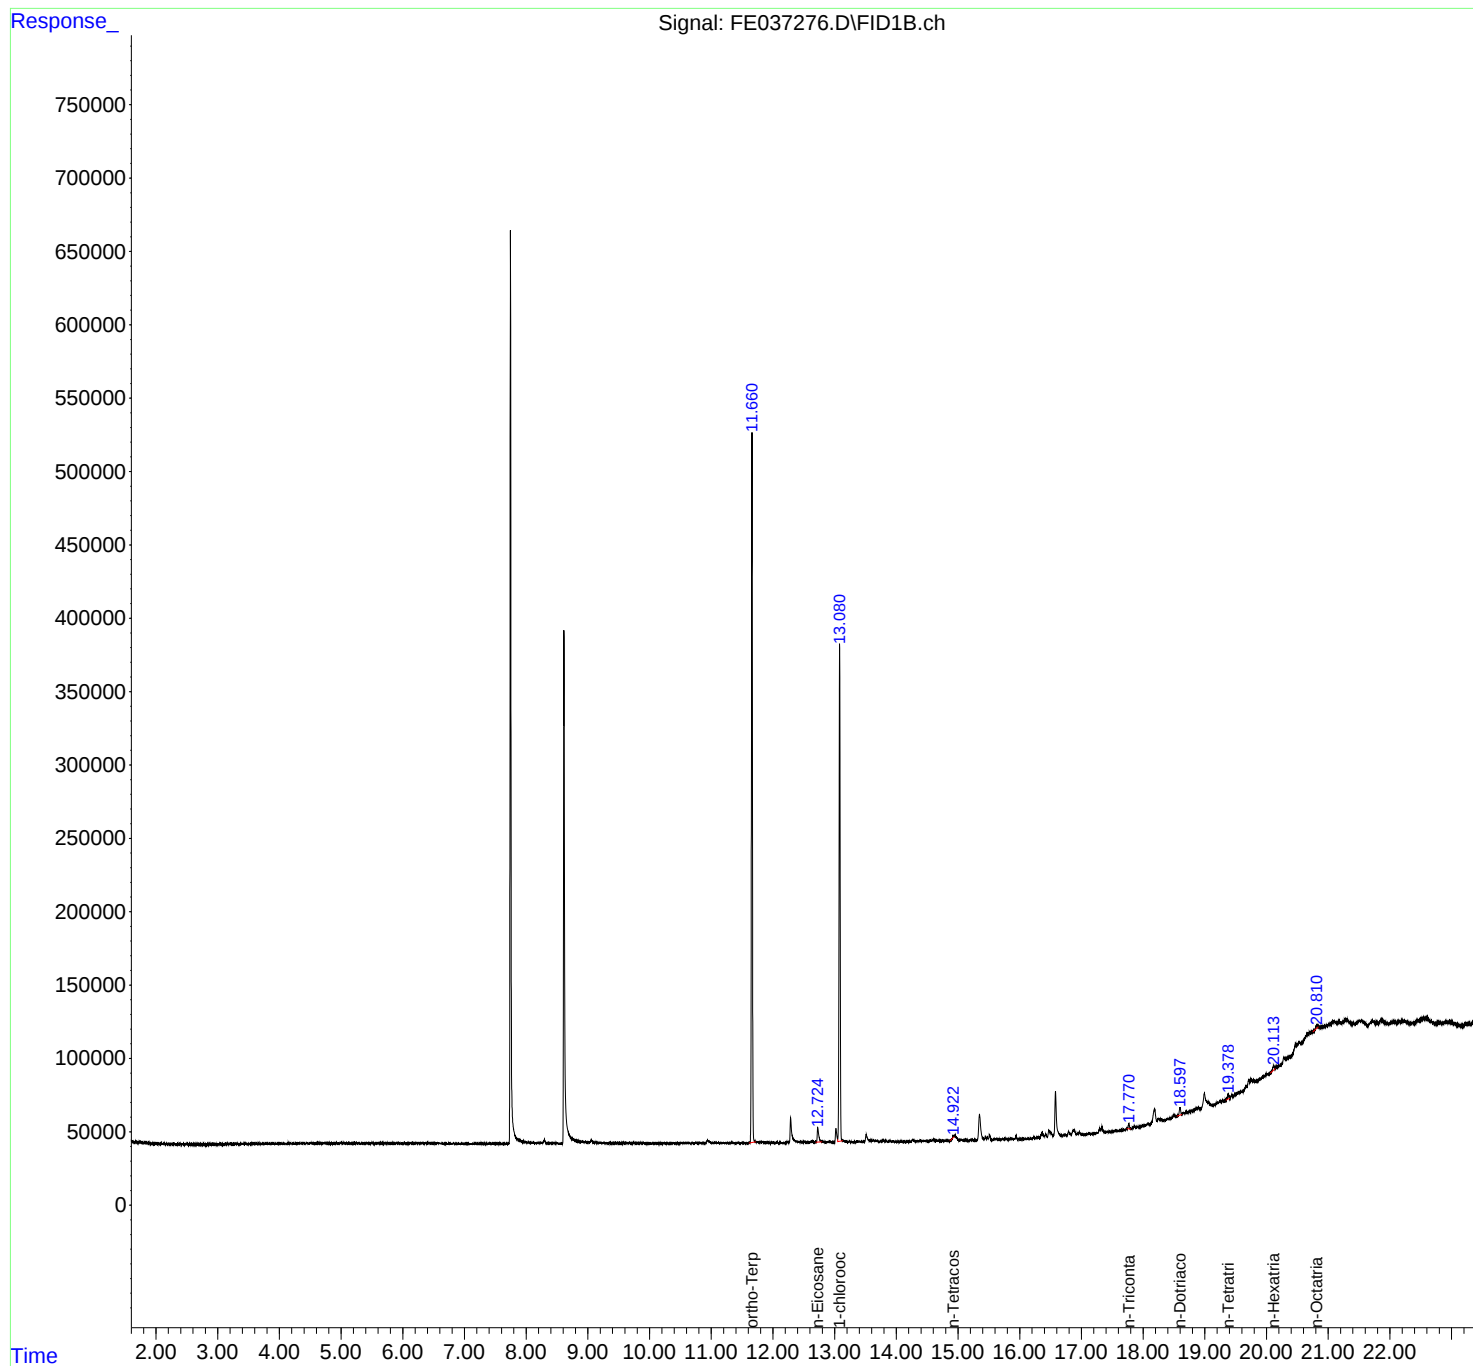


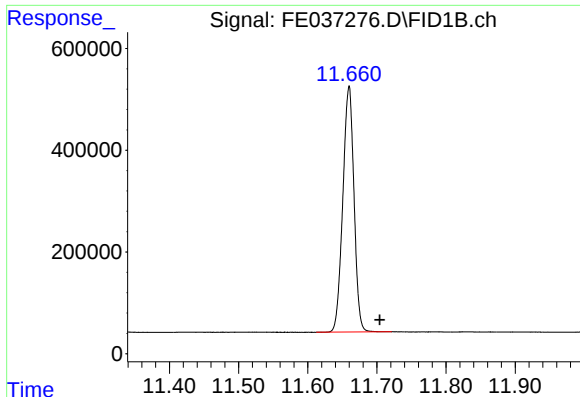

#9 ortho-Terphenyl (SURR)


R.T.: 11.660 min
Delta R.T.: -0.044 min
Response: 5428833
Conc: 31.41 ug/ml

Instrument :
FID_E
ClientSampleId :

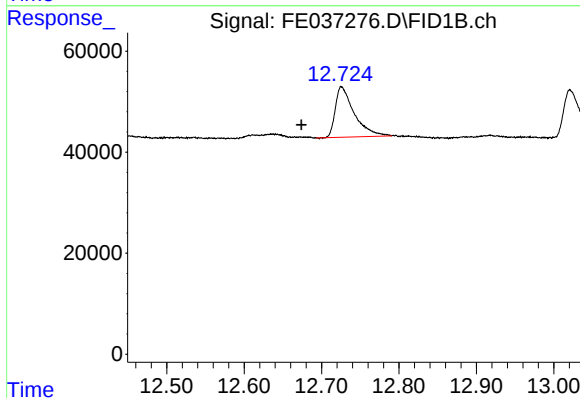


#10 n-Eicosane (C20)

R.T.: 12.726 min
Delta R.T.: 0.052 min
Response: 169075
Conc: 1.03 ug/ml

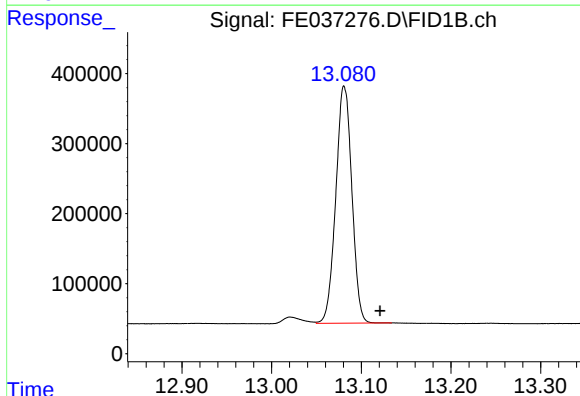


#12 1-chlorooctadecane (SURR)

R.T.: 13.081 min
Delta R.T.: -0.040 min
Response: 4216900
Conc: 30.86 ug/ml

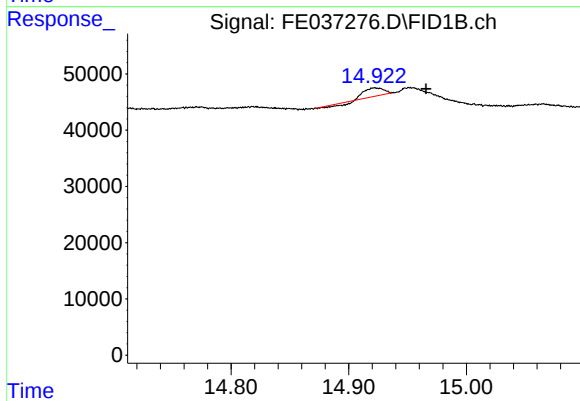

#14 n-Tetracosane (C24)


R.T.: 14.922 min
Delta R.T.: -0.044 min
Response: 12492
Conc: 0.08 ug/ml

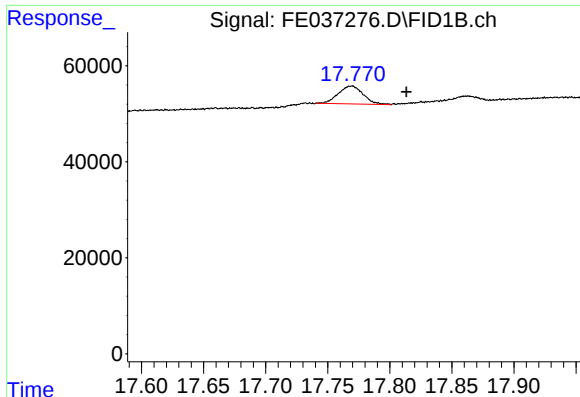

#17 n-Tricontane (C30)


R.T.: 17.769 min
Delta R.T.: -0.044 min
Response: 51958
Conc: 0.33 ug/ml

Instrument :
FID_E
ClientSampleId :

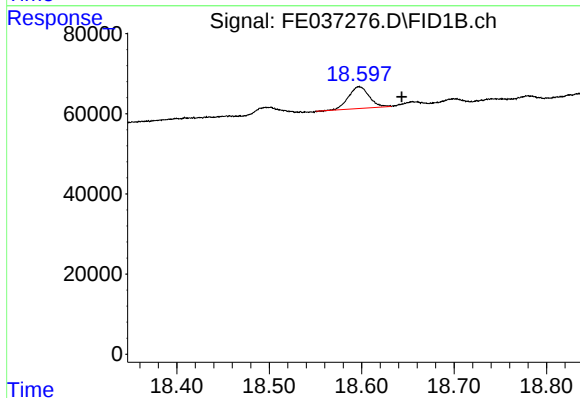


#18 n-Dotriacontane (C32)

R.T.: 18.597 min
Delta R.T.: -0.046 min
Response: 84066
Conc: 0.56 ug/ml

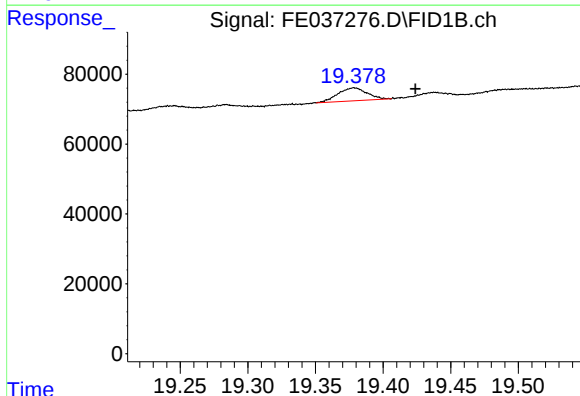


#19 n-Tetratriacontane (C34)

R.T.: 19.378 min
Delta R.T.: -0.046 min
Response: 55800
Conc: 0.42 ug/ml

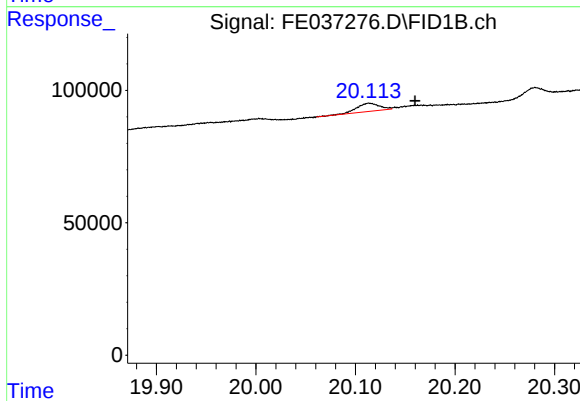

#20 n-Hexatriacontane (C36)

R.T.: 20.114 min
Delta R.T.: -0.046 min
Response: 49431
Conc: 0.39 ug/ml

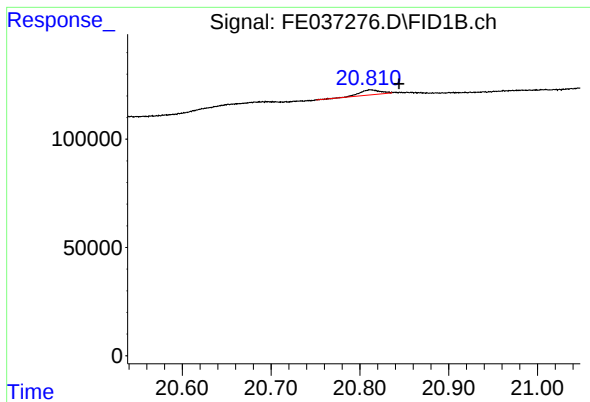

#21 n-Octatriacontane (C38)

R.T.: 20.812 min
Delta R.T.: -0.032 min
Response: 36379
Conc: 0.30 ug/ml

Instrument :
FID_E
ClientSampleId :