

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082622AL\
 Data File : FE037277.D
 Signal(s) : FID1B.ch
 Acq On : 26 Aug 2022 17:59
 Operator : YP\AJ
 Sample : N4375-07D
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 27 02:42:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082322.M
 Quant Title : GC Extractables
 QLast Update : Sat Aug 27 02:21:03 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.660	5388036	31.177 ug/ml
Spiked Amount 50.000		Recovery =	62.35%
12) S 1-chlorooctadecane (S...	13.081	4186578	30.642 ug/ml
Spiked Amount 50.000		Recovery =	61.28%
Target Compounds			
10) T n-Eicosane (C20)	12.725f	174078	1.057 ug/ml
14) T n-Tetracosane (C24)	14.919	7666	0.046 ug/ml
16) T n-Octacosane (C28)	16.884	80242	0.505 ug/ml
18) T n-Dotriacontane (C32)	18.596	63027	0.423 ug/ml
20) T n-Hexatriacontane (C36)	20.114	31020	0.242 ug/ml
21) T n-Octatriacontane (C38)	20.813	75172	0.626 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082622AL\
Data File : FE037277.D
Signal(s) : FID1B.ch
Acq On : 26 Aug 2022 17:59
Operator : YP\AJ
Sample : N4375-07D
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 27 02:42:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082322.M
Quant Title : GC Extractables
QLast Update : Sat Aug 27 02:21:03 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

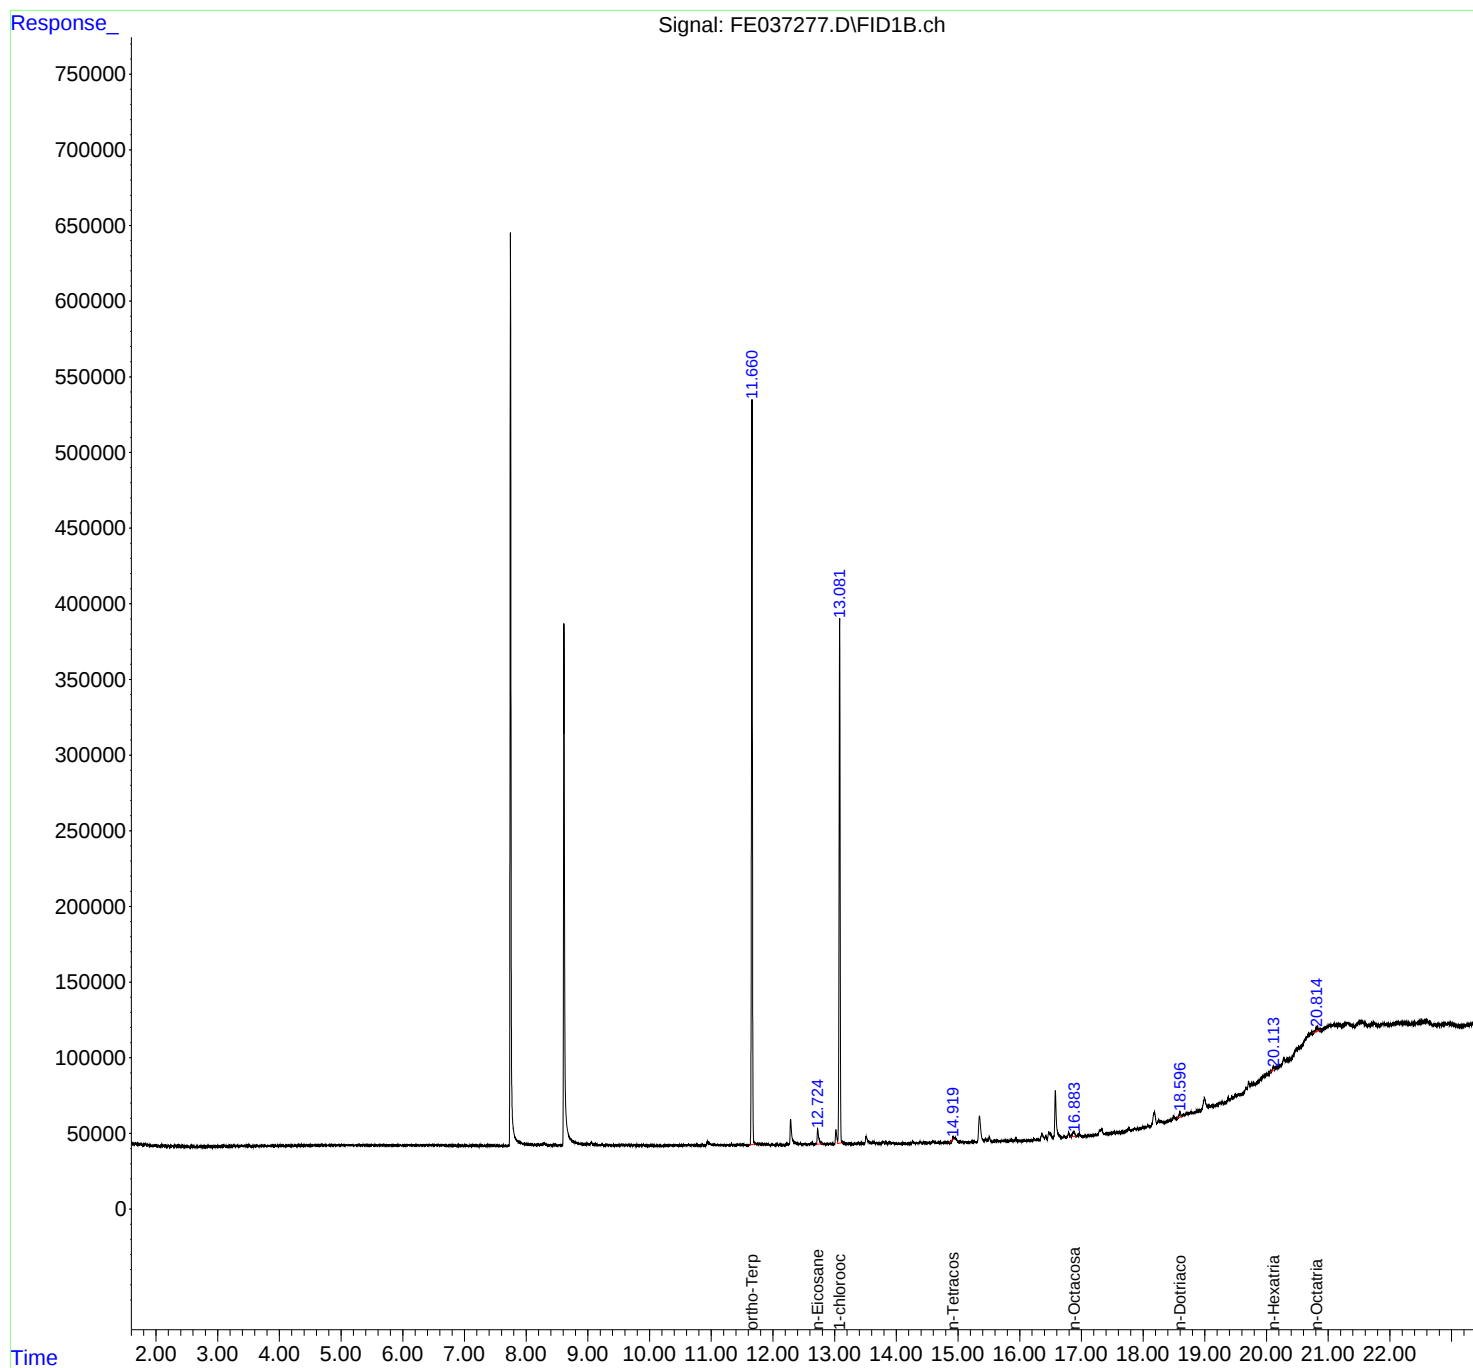


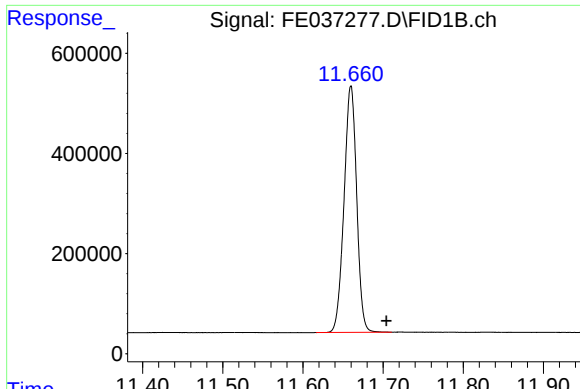

#9 ortho-Terphenyl (SURR)


R.T.: 11.660 min
Delta R.T.: -0.044 min
Response: 5388036
Conc: 31.18 ug/ml

Instrument :
FID_E
ClientSampleId :

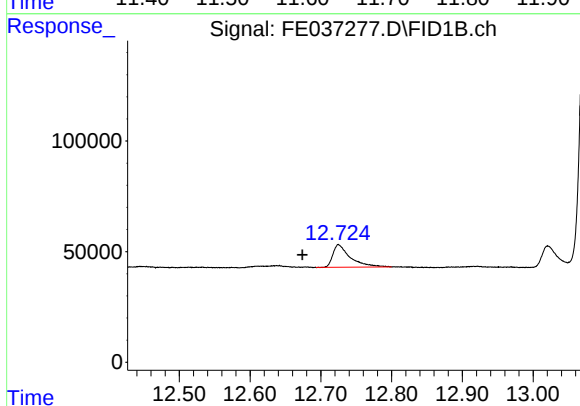


#10 n-Eicosane (C20)

R.T.: 12.725 min
Delta R.T.: 0.051 min
Response: 174078
Conc: 1.06 ug/ml

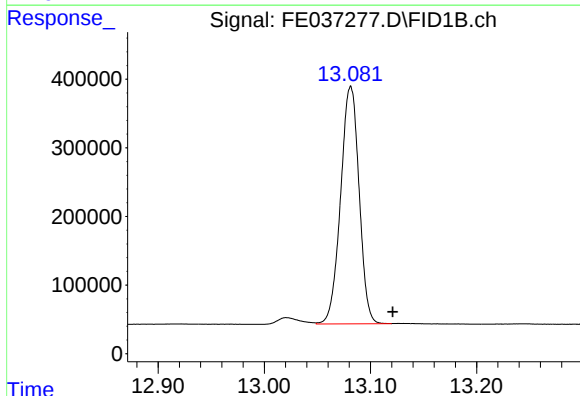


#12 1-chlorooctadecane (SURR)

R.T.: 13.081 min
Delta R.T.: -0.039 min
Response: 4186578
Conc: 30.64 ug/ml

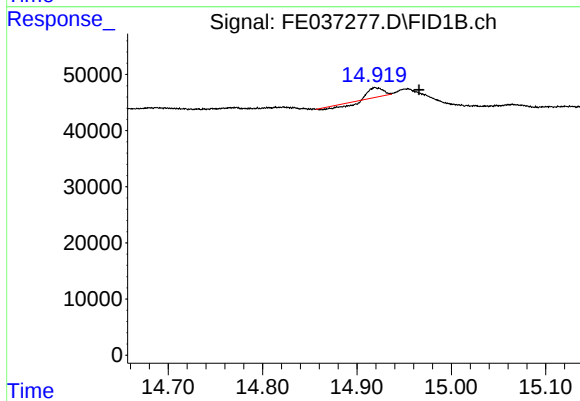

#14 n-Tetracosane (C24)


R.T.: 14.919 min
Delta R.T.: -0.047 min
Response: 7666
Conc: 0.05 ug/ml

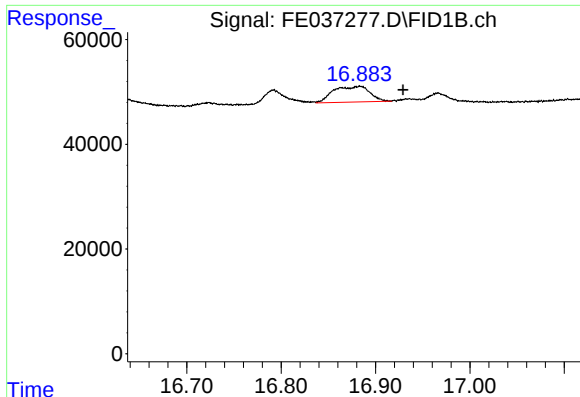

#16 n-Octacosane (C28)


R.T.: 16.884 min
Delta R.T.: -0.046 min
Response: 80242
Conc: 0.51 ug/ml

Instrument :
FID_E
ClientSampleId :

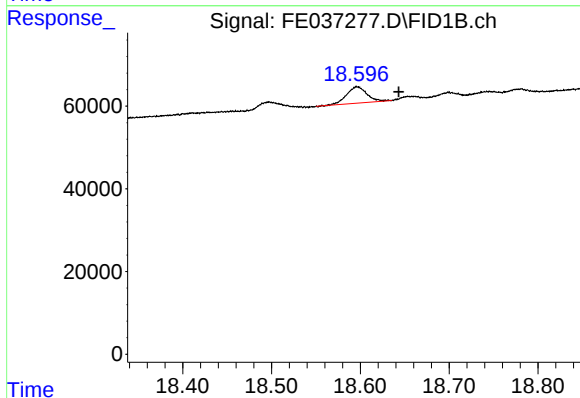


#18 n-Dotriacontane (C32)

R.T.: 18.596 min
Delta R.T.: -0.047 min
Response: 63027
Conc: 0.42 ug/ml

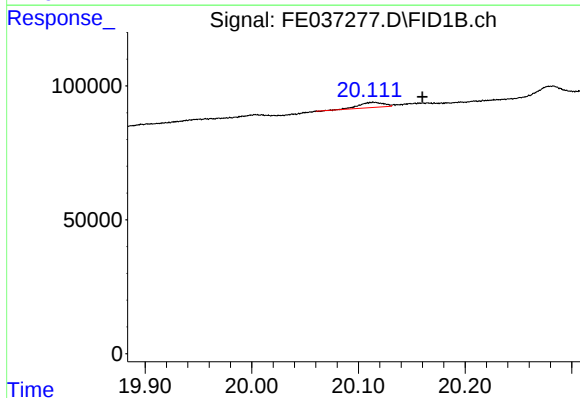

#20 n-Hexatriacontane (C36)

R.T.: 20.114 min
Delta R.T.: -0.046 min
Response: 31020
Conc: 0.24 ug/ml

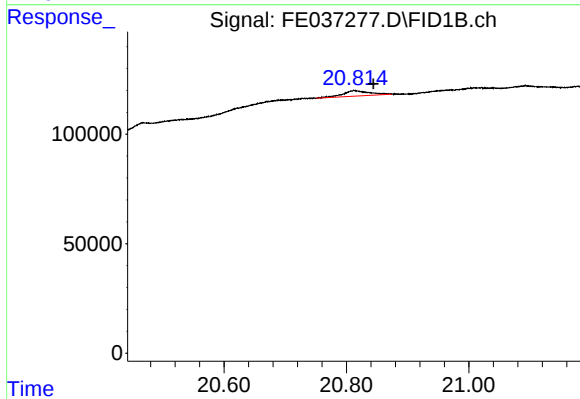

#21 n-Octatriacontane (C38)

R.T.: 20.813 min
Delta R.T.: -0.031 min
Response: 75172
Conc: 0.63 ug/ml