

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE082624AL\  
 Data File : FE049752.D  
 Signal(s) : FID1B.ch  
 Acq On : 26 Aug 2024 09:50  
 Operator : YP\AJ  
 Sample : P3714-01DL 5X  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 EO-01-08222024DL

Integration File: autoint1.e  
 Quant Time: Aug 27 01:20:40 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 081424.M  
 Quant Title : GC Extractables  
 QLast Update : Wed Aug 14 11:05:17 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units  |
|--------------------------------|--------|------------|-------------|
| -----                          |        |            |             |
| System Monitoring Compounds    |        |            |             |
| 9) S ortho-Terphenyl (SURR)    | 11.884 | 775930     | 4.798 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 9.60%       |
| 12) S 1-chlorooctadecane (S... | 13.318 | 687306     | 5.633 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 11.27%      |

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE082624AL\  
Data File : FE049752.D  
Signal(s) : FID1B.ch  
Acq On : 26 Aug 2024 09:50  
Operator : YP\AJ  
Sample : P3714-01DL 5X  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
EO-01-08222024DL

Integration File: autoint1.e  
Quant Time: Aug 27 01:20:40 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 081424.M  
Quant Title : GC Extractables  
QLast Update : Wed Aug 14 11:05:17 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

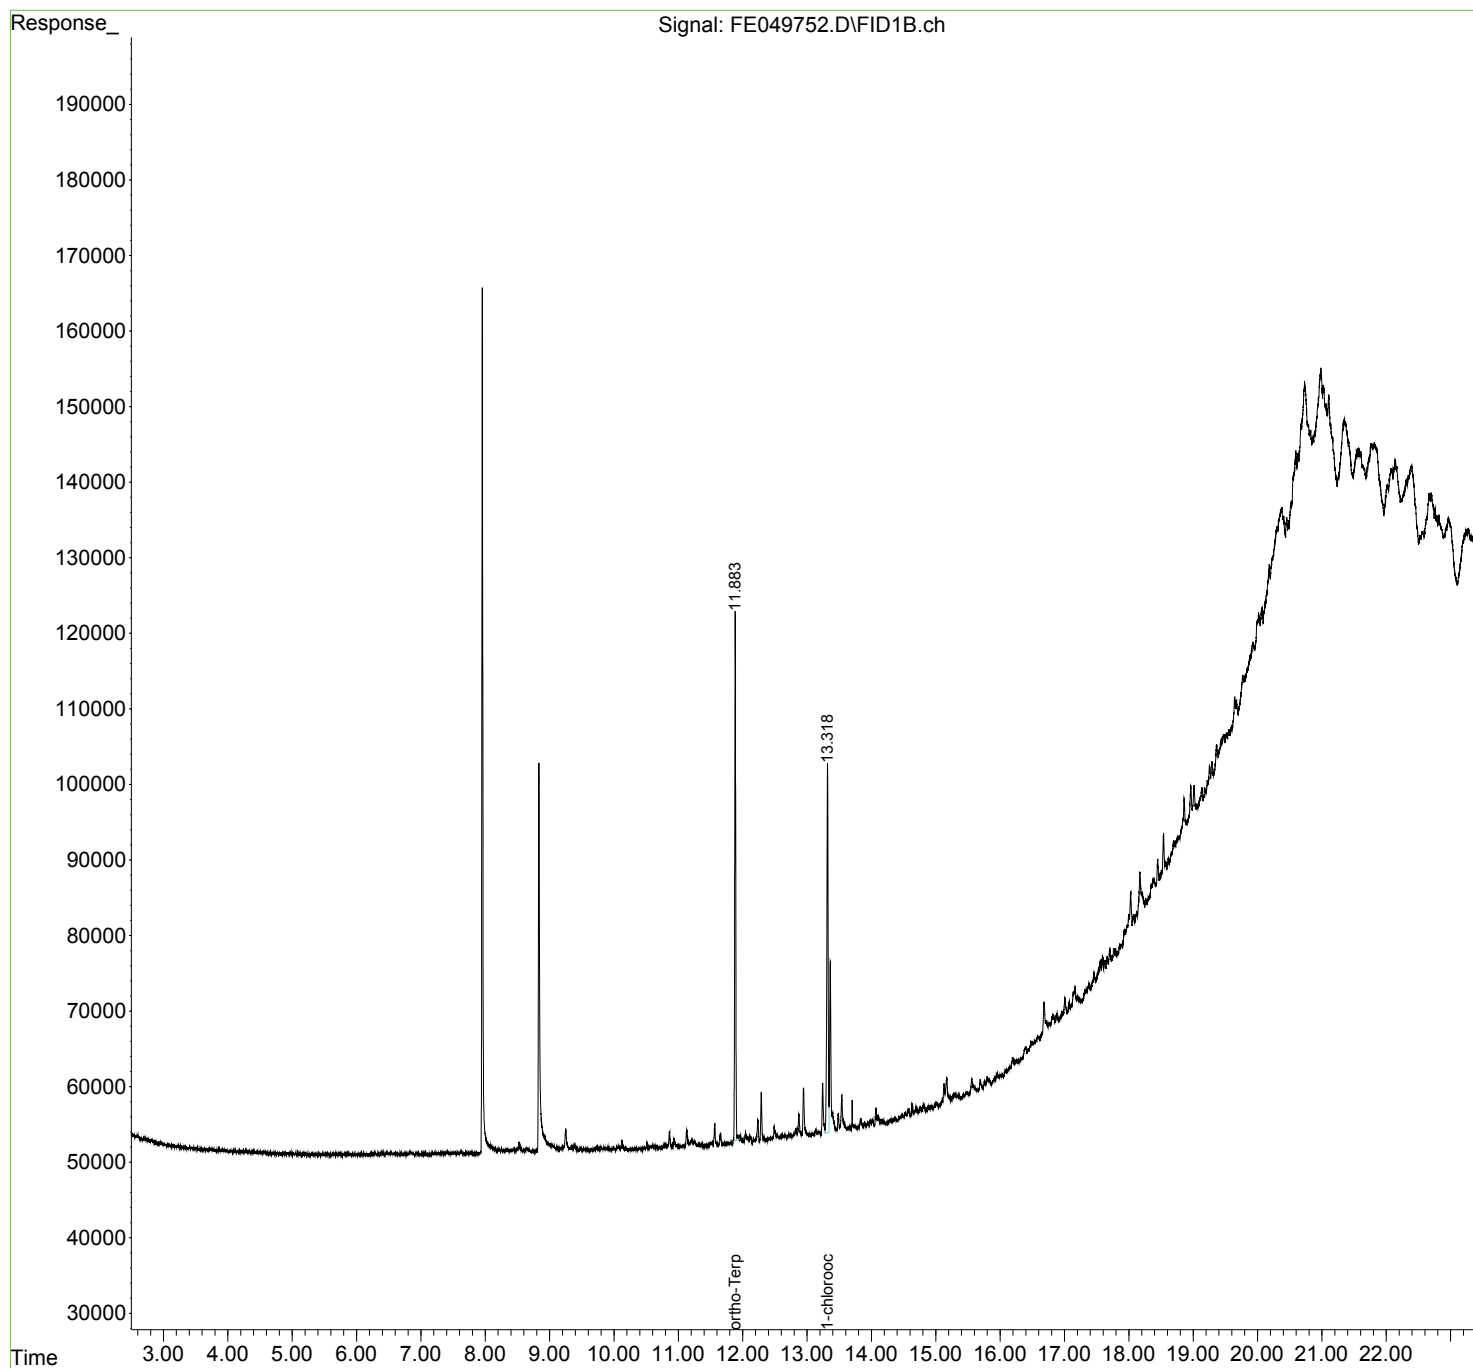

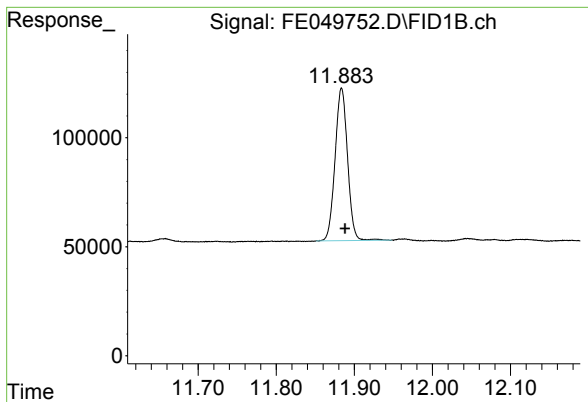

#9 ortho-Terphenyl (SURR)


R.T.: 11.884 min  
Delta R.T.: -0.005 min  
Response: 775930  
Conc: 4.80 ug/ml

Instrument :

FID\_E

ClientSampleId :

EO-01-08222024DL

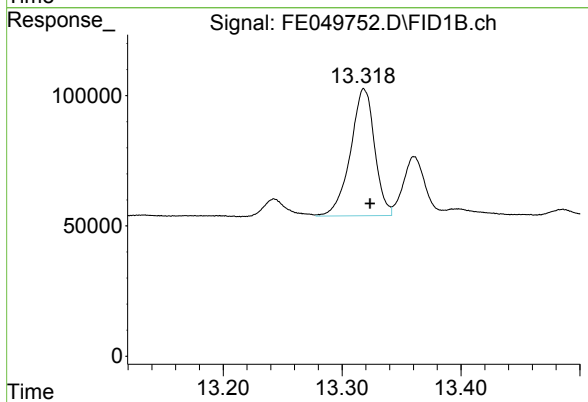

#12 1-chlorooctadecane (SURR)

R.T.: 13.318 min  
Delta R.T.: -0.005 min  
Response: 687306  
Conc: 5.63 ug/ml