

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE082725AL\  
Data File : FE055529.D  
Signal(s) : FID1B.ch  
Acq On : 27 Aug 2025 07:51  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Aug 27 11:17:22 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 080125.M  
Quant Title : GC Extractables  
QLast Update : Fri Aug 01 13:47:09 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

| Compound | R.T. | Response | Conc Units |
|----------|------|----------|------------|
|----------|------|----------|------------|

-----  
System Monitoring Compounds

Target Compounds

|       |                          |        |        |             |
|-------|--------------------------|--------|--------|-------------|
| 17) T | n-Tricontane (C30)       | 18.242 | 134399 | 1.092 ug/ml |
| 18) T | n-Dotriacontane (C32)    | 19.077 | 223717 | 1.834 ug/ml |
| 19) T | n-Tetratriacontane (C34) | 19.861 | 220564 | 1.886 ug/ml |
| 20) T | n-Hexatriacontane (C36)  | 20.603 | 156555 | 1.432 ug/ml |

-----  
(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE082725AL\  
Data File : FE055529.D  
Signal(s) : FID1B.ch  
Acq On : 27 Aug 2025 07:51  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Aug 27 11:17:22 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 080125.M  
Quant Title : GC Extractables  
QLast Update : Fri Aug 01 13:47:09 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

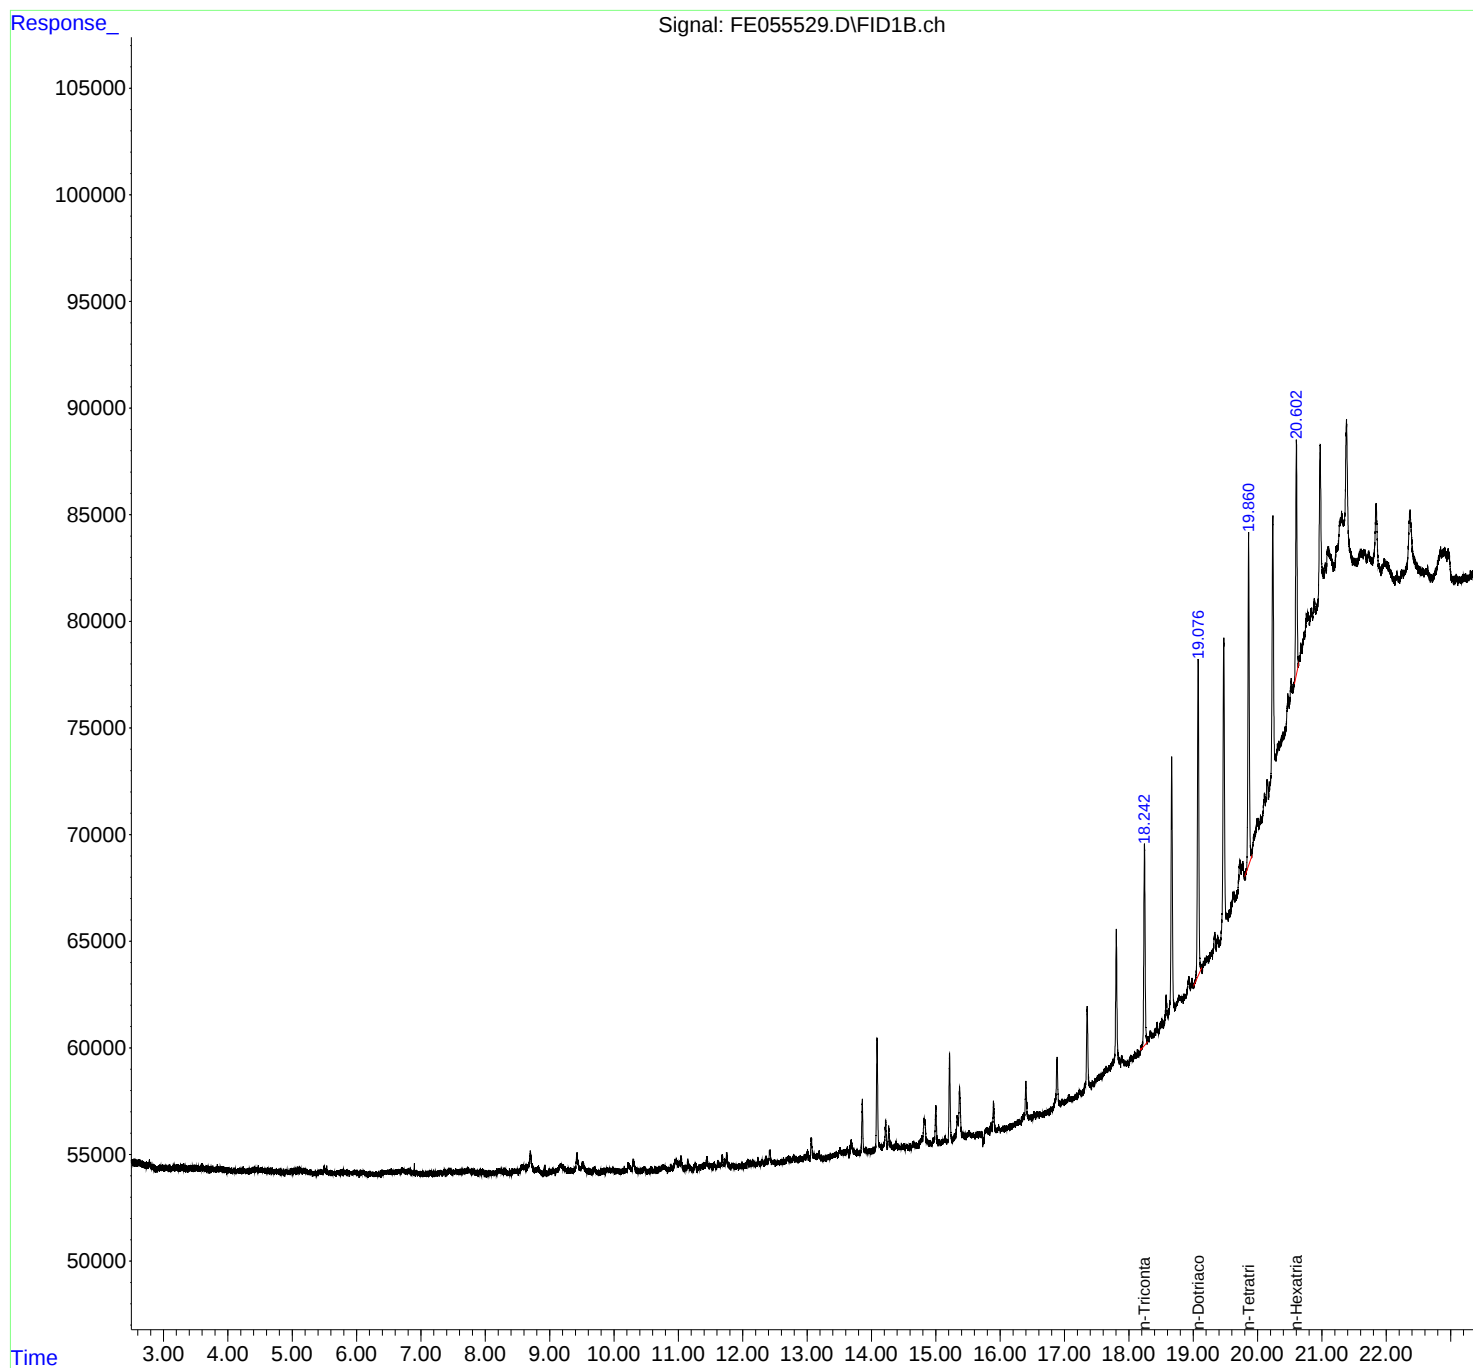


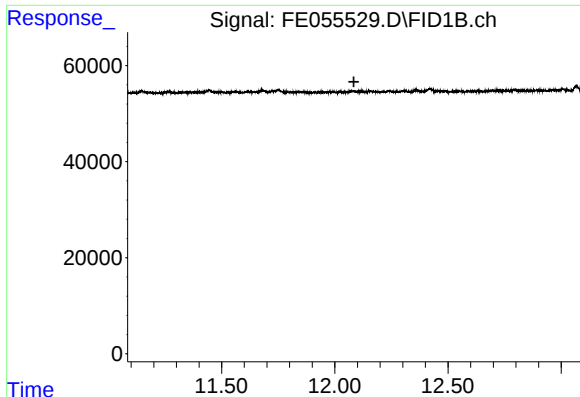

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min  
Exp R.T.: 12.084 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_E  
ClientSampleId :

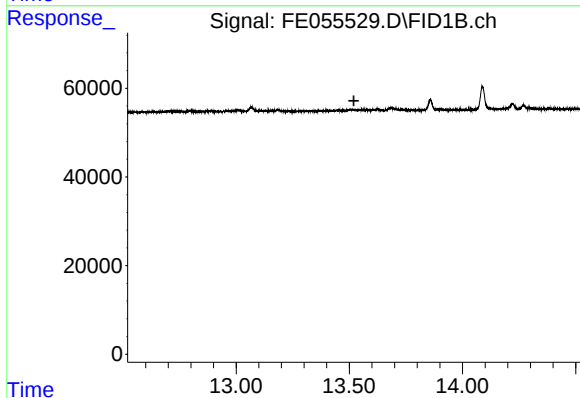


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min  
Exp R.T.: 13.520 min  
Response: 0  
Conc: N.D.

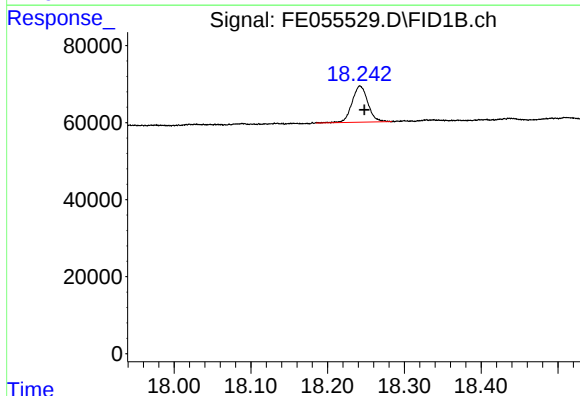


#17 n-Tricontane (C30)

R.T.: 18.242 min  
Delta R.T.: -0.006 min  
Response: 134399  
Conc: 1.09 ug/ml

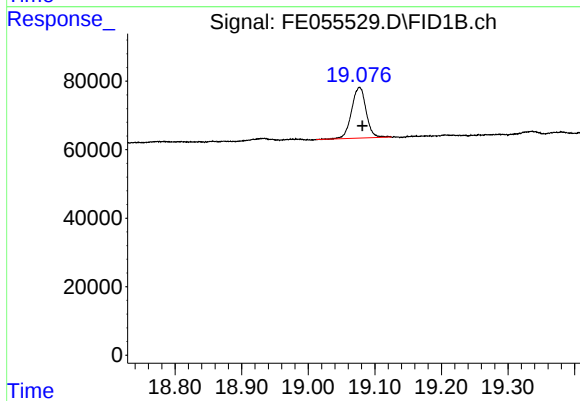

#18 n-Dotriacontane (C32)


R.T.: 19.077 min  
Delta R.T.: -0.005 min  
Response: 223717  
Conc: 1.83 ug/ml

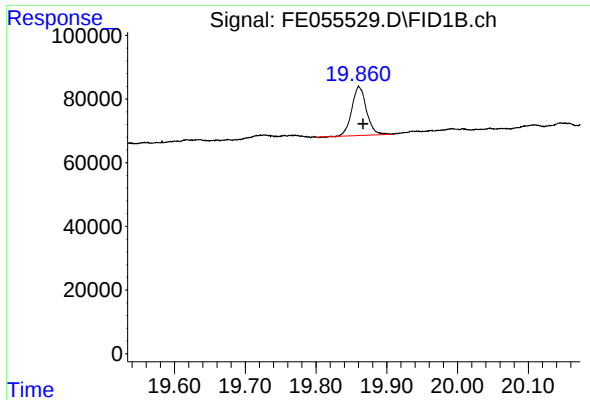

#19 n-Tetratriacontane (C34)

R.T.: 19.861 min  
Delta R.T.: -0.006 min  
Response: 220564  
Conc: 1.89 ug/ml

Instrument :  
FID\_E  
ClientSampleId :

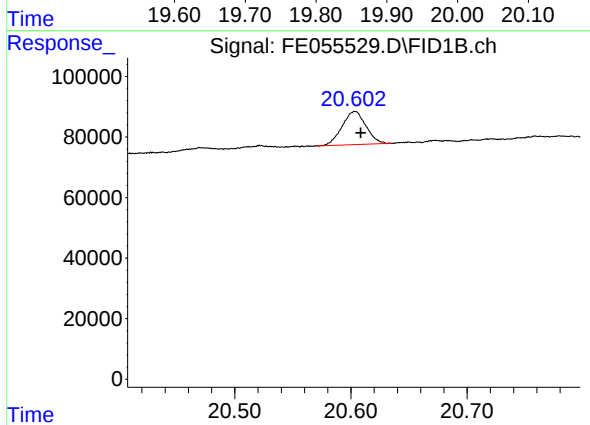

#20 n-Hexatriacontane (C36)

R.T.: 20.603 min  
Delta R.T.: -0.005 min  
Response: 156555  
Conc: 1.43 ug/ml