

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082725\
Data File : FF016232.D
Signal(s) : FID2B.ch
Acq On : 27 Aug 2025 08:42
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Aug 28 02:30:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080625.M
Quant Title :
QLast Update : Wed Aug 06 13:50:48 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	15.078	2178816	19.520 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.982	47698	0.383 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF082725\
Data File : FF016232.D
Signal(s) : FID2B.ch
Acq On : 27 Aug 2025 08:42
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Aug 28 02:30:39 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF080625.M
Quant Title :
QLast Update : Wed Aug 06 13:50:48 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

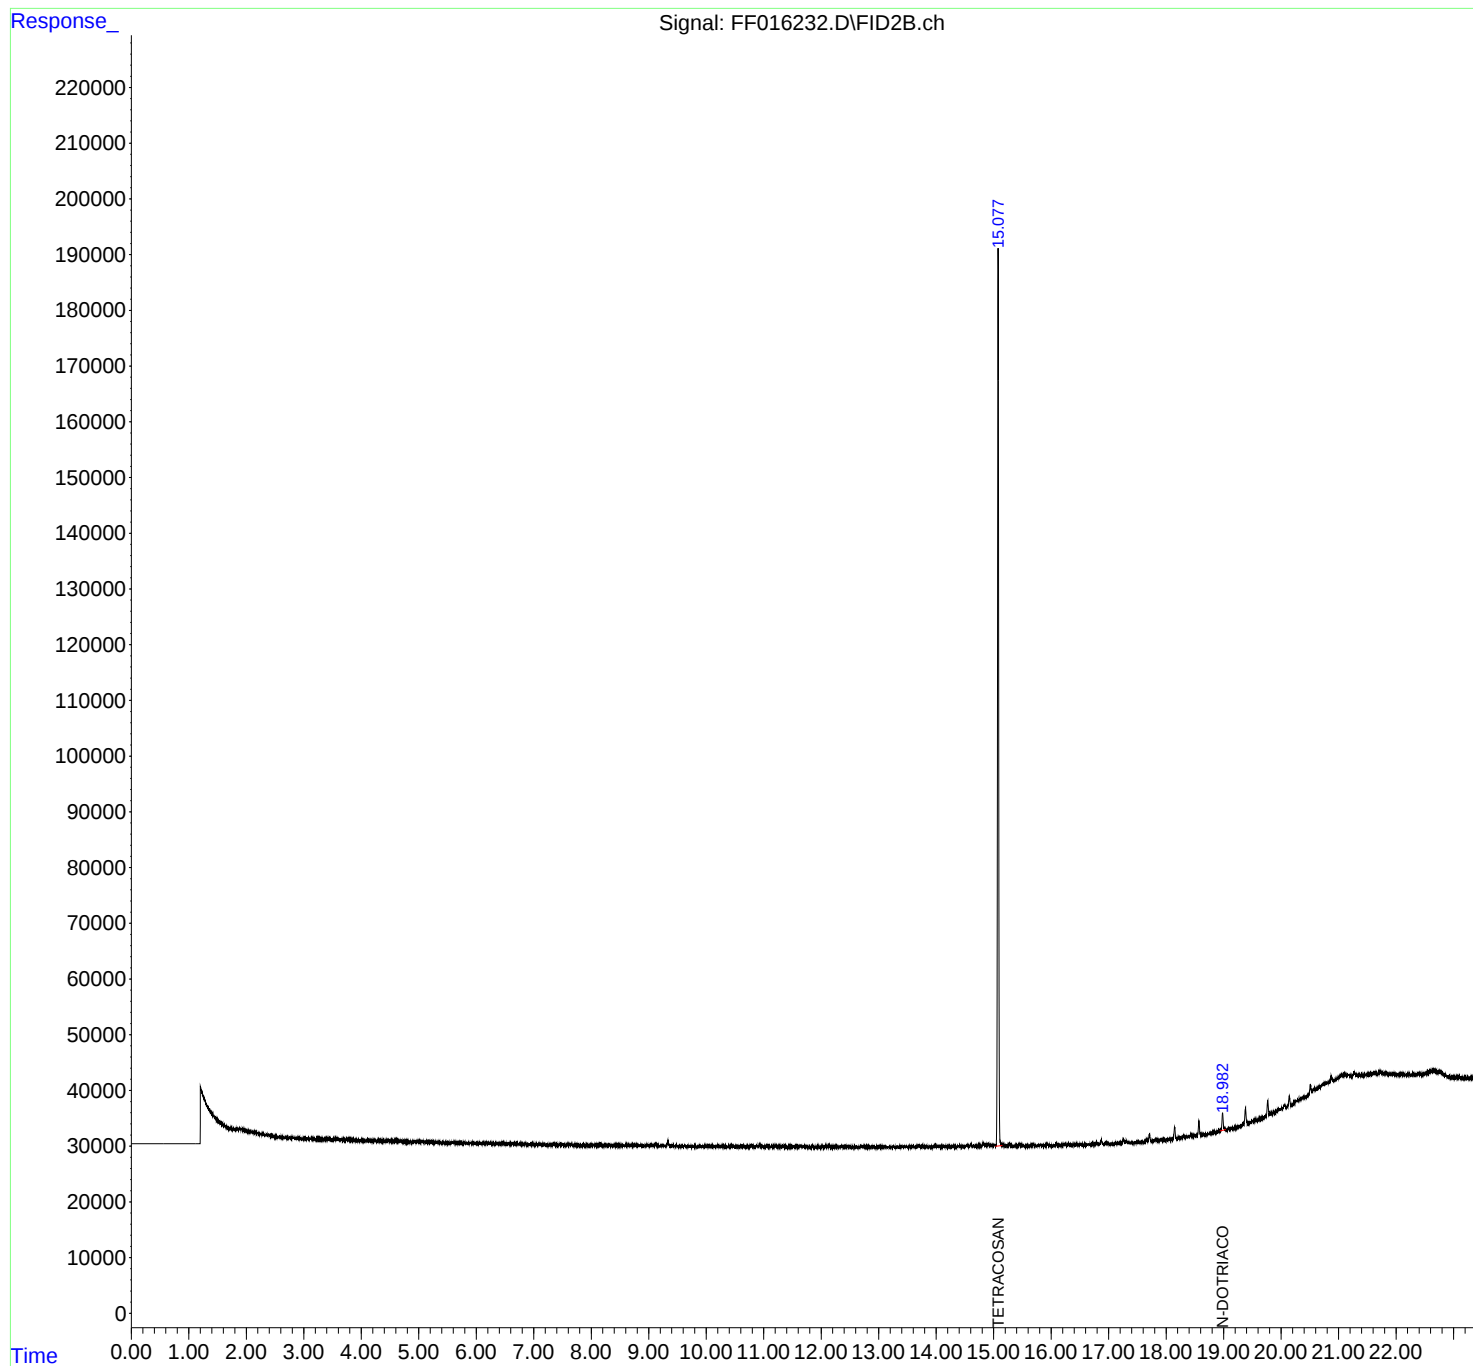


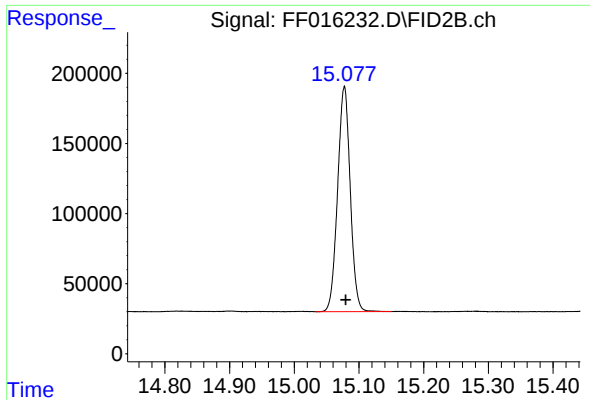

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.078 min
Delta R.T.: -0.002 min
Response: 2178816
Conc: 19.52 ug/ml

Instrument :
FID_E
ClientSampleId :
I.BLK

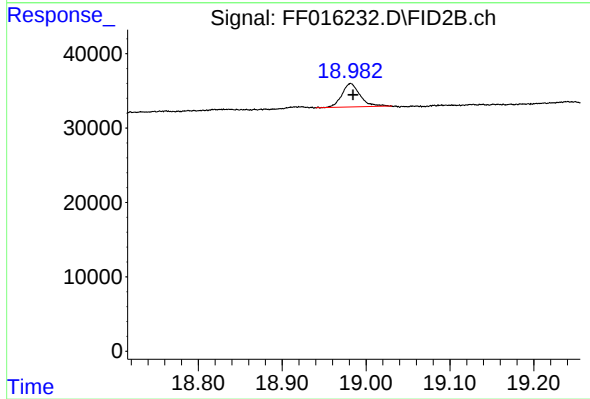

#14 N-DOTRIACONTANE

R.T.: 18.982 min
Delta R.T.: -0.003 min
Response: 47698
Conc: 0.38 ug/ml