

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082820\
Data File : FE032618.D
Signal(s) : FID1B.CH
Acq On : 28 Aug 2020 8:37
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Aug 31 00:52:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE081120.M
Quant Title :
QLast Update : Thu Aug 13 11:46:52 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.592	220940	0.627 ug/ml
16)	N-HEXATRIACONTANE	20.146	538730	2.390 ug/ml
18)	N-TETRACONTANE	21.821	1038089	6.229 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082820\
Data File : FE032618.D
Signal(s) : FID1B.CH
Acq On : 28 Aug 2020 8:37
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Aug 31 00:52:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE081120.M
Quant Title :
QLast Update : Thu Aug 13 11:46:52 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

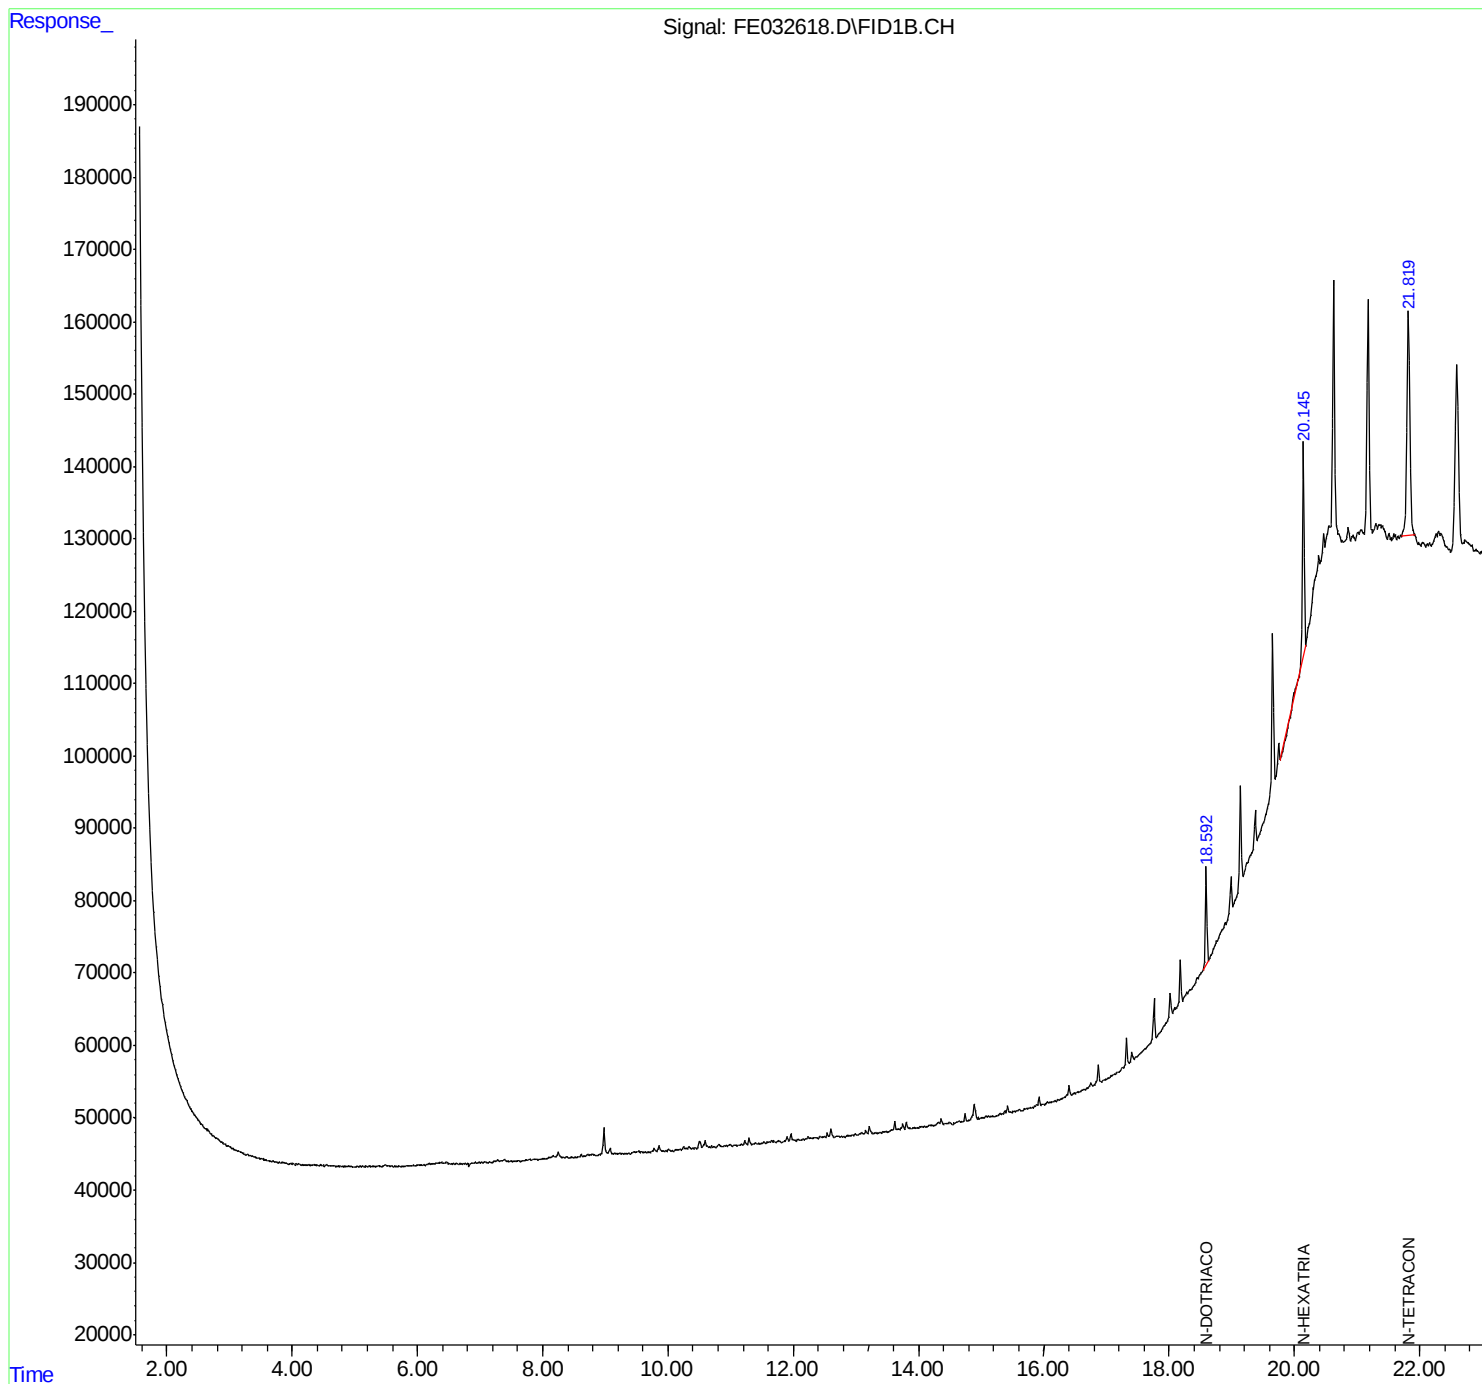


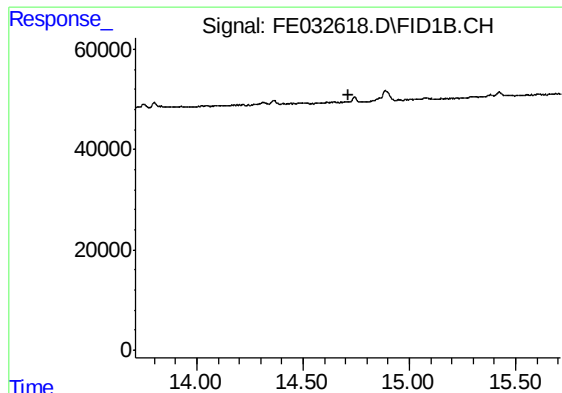

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.711 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
MECL2

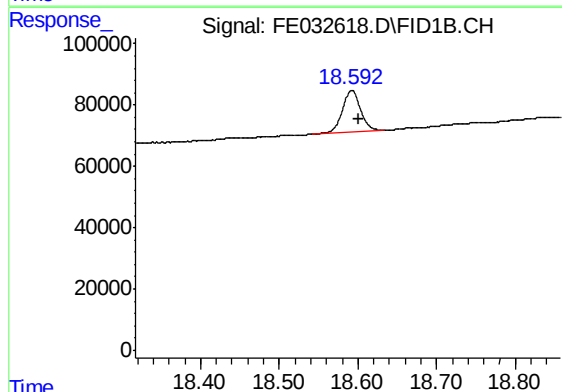


#14 N-DOTRIACONTANE

R.T.: 18.592 min
Delta R.T.: -0.009 min
Response: 220940
Conc: 0.63 ug/ml

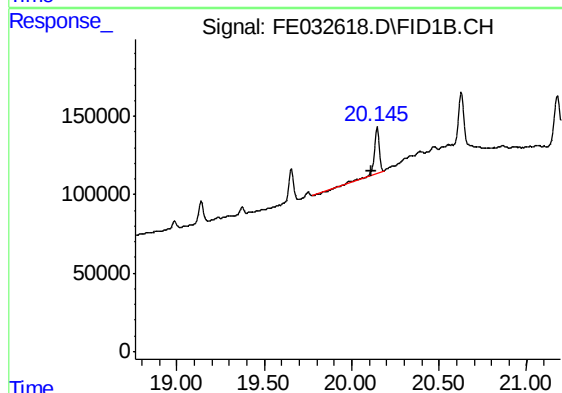

#16 N-HEXATRIACONTANE

R.T.: 20.146 min
Delta R.T.: 0.029 min
Response: 538730
Conc: 2.39 ug/ml

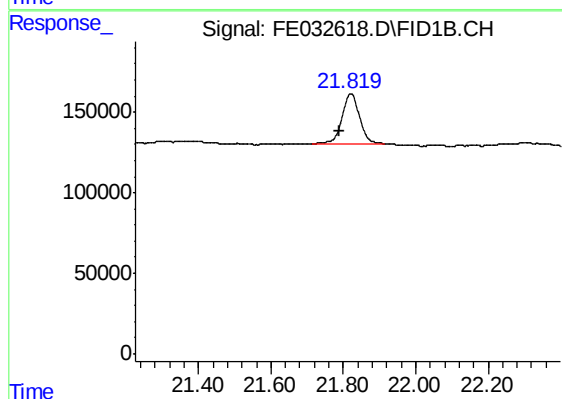

#18 N-TETRACONTANE

R.T.: 21.821 min
Delta R.T.: 0.033 min
Response: 1038089
Conc: 6.23 ug/ml