

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082820\
 Data File : FE032635.D
 Signal(s) : FID1B.CH
 Acq On : 28 Aug 2020 20:25
 Operator : DD\AJ
 Sample : L3832-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 SIMW-02-20200827

Integration File: autoint1.e
 Quant Time: Aug 31 00:56:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE081120.M
 Quant Title :
 QLast Update : Thu Aug 13 11:46:52 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.698	6131210	19.051 ug/ml
Target Compounds			
4) N-TETRADECANE	8.313	1488752	4.122 ug/ml
12) N-OCTACOSANE	16.866	207975	0.558 ug/ml
13) N-TRIACONTANE	17.752	306340	0.821 ug/ml
14) N-DOTRIACONTANE	18.582	158032	0.448 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082820\
Data File : FE032635.D
Signal(s) : FID1B.CH
Acq On : 28 Aug 2020 20:25
Operator : DD\AJ
Sample : L3832-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
SIMW-02-20200827

Integration File: autoint1.e
Quant Time: Aug 31 00:56:03 2020
Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE081120.M
Quant Title :
QLast Update : Thu Aug 13 11:46:52 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

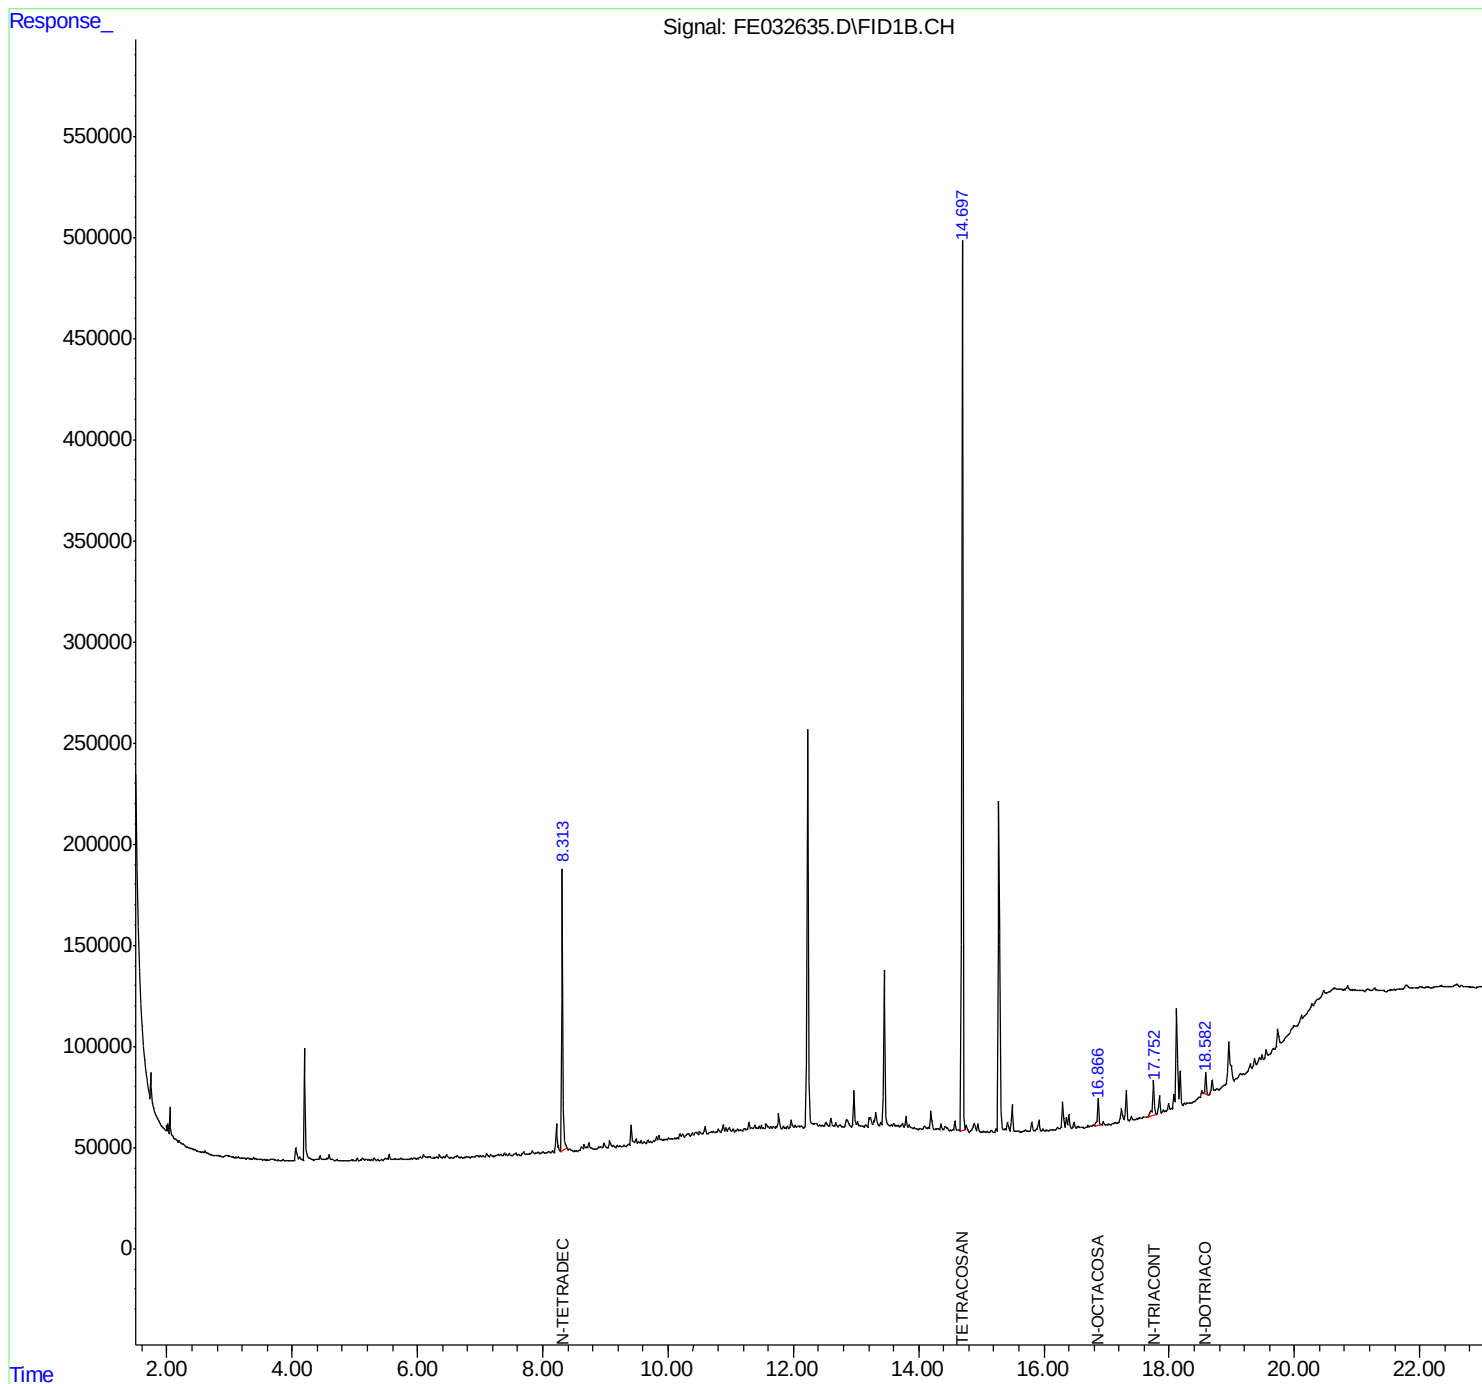


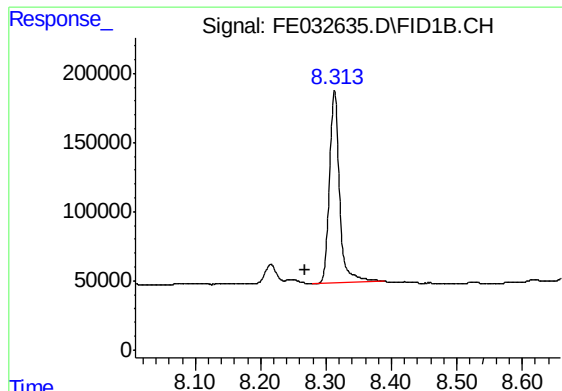

#4 N-TETRADECANE


R.T.: 8.313 min
Delta R.T.: 0.044 min
Response: 1488752
Conc: 4.12 ug/ml

Instrument :
FID_E
ClientSampleId :
SIMW-02-20200827

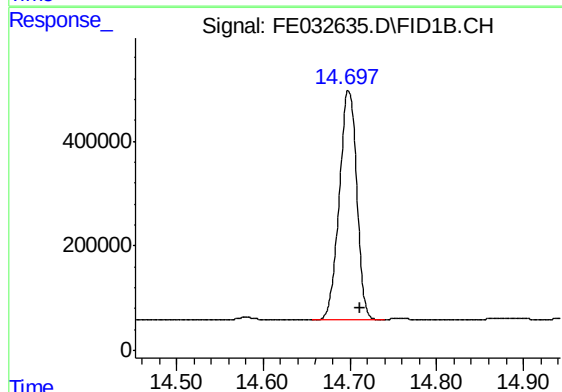


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.698 min
Delta R.T.: -0.013 min
Response: 6131210
Conc: 19.05 ug/ml

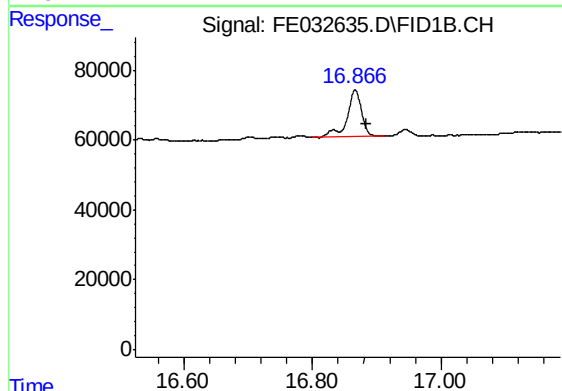


#12 N-OCTACOSANE

R.T.: 16.866 min
Delta R.T.: -0.018 min
Response: 207975
Conc: 0.56 ug/ml

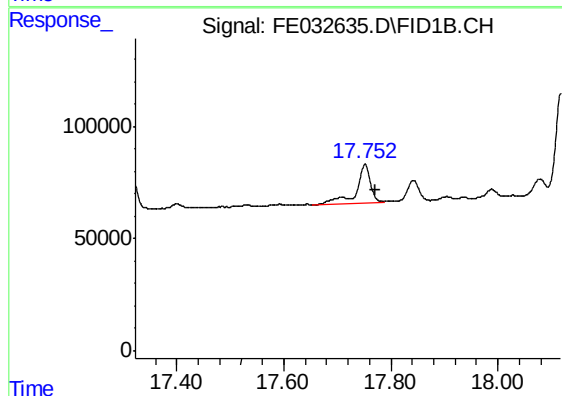

#13 N-TRIACONTANE

R.T.: 17.752 min
Delta R.T.: -0.019 min
Response: 306340
Conc: 0.82 ug/ml

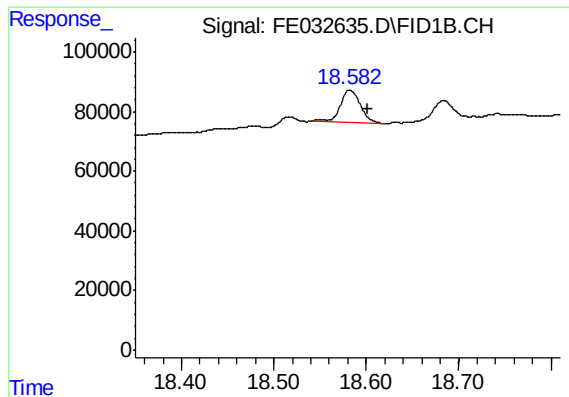

#14 N-DOTRIACONTANE

R.T.: 18.582 min
Delta R.T.: -0.019 min
Response: 158032
Conc: 0.45 ug/ml

Instrument :
FID_E
ClientSampleId :
SIMW-02-20200827