

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082820\
 Data File : FE032642.D
 Signal(s) : FID1B.CH
 Acq On : 29 Aug 2020 00:20
 Operator : DD\AJ
 Sample : L3832-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 SIMW-07-20200827

Integration File: autoint1.e
 Quant Time: Aug 31 00:57:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE081120.M
 Quant Title :
 QLast Update : Thu Aug 13 11:46:52 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.700	7586162	23.572 ug/ml
Target Compounds			
5) N-HEXADECANE	9.876	110138	0.302 ug/ml
6) N-OCTADECANE	11.276	551105	1.484 ug/ml
7) N-EICOSANE	12.631	24741	0.067 ug/ml
14) N-DOTRIACONTANE	18.582	150882	0.428 ug/ml
15) N-TETRATRIACONTANE	19.365	90194	0.305 ug/ml
16) N-HEXATRIACONTANE	20.105	36646	0.163 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE082820\
Data File : FE032642.D
Signal(s) : FID1B.CH
Acq On : 29 Aug 2020 00:20
Operator : DD\AJ
Sample : L3832-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
SIMW-07-20200827

Integration File: autoint1.e
Quant Time: Aug 31 00:57:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE081120.M
Quant Title :
QLast Update : Thu Aug 13 11:46:52 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

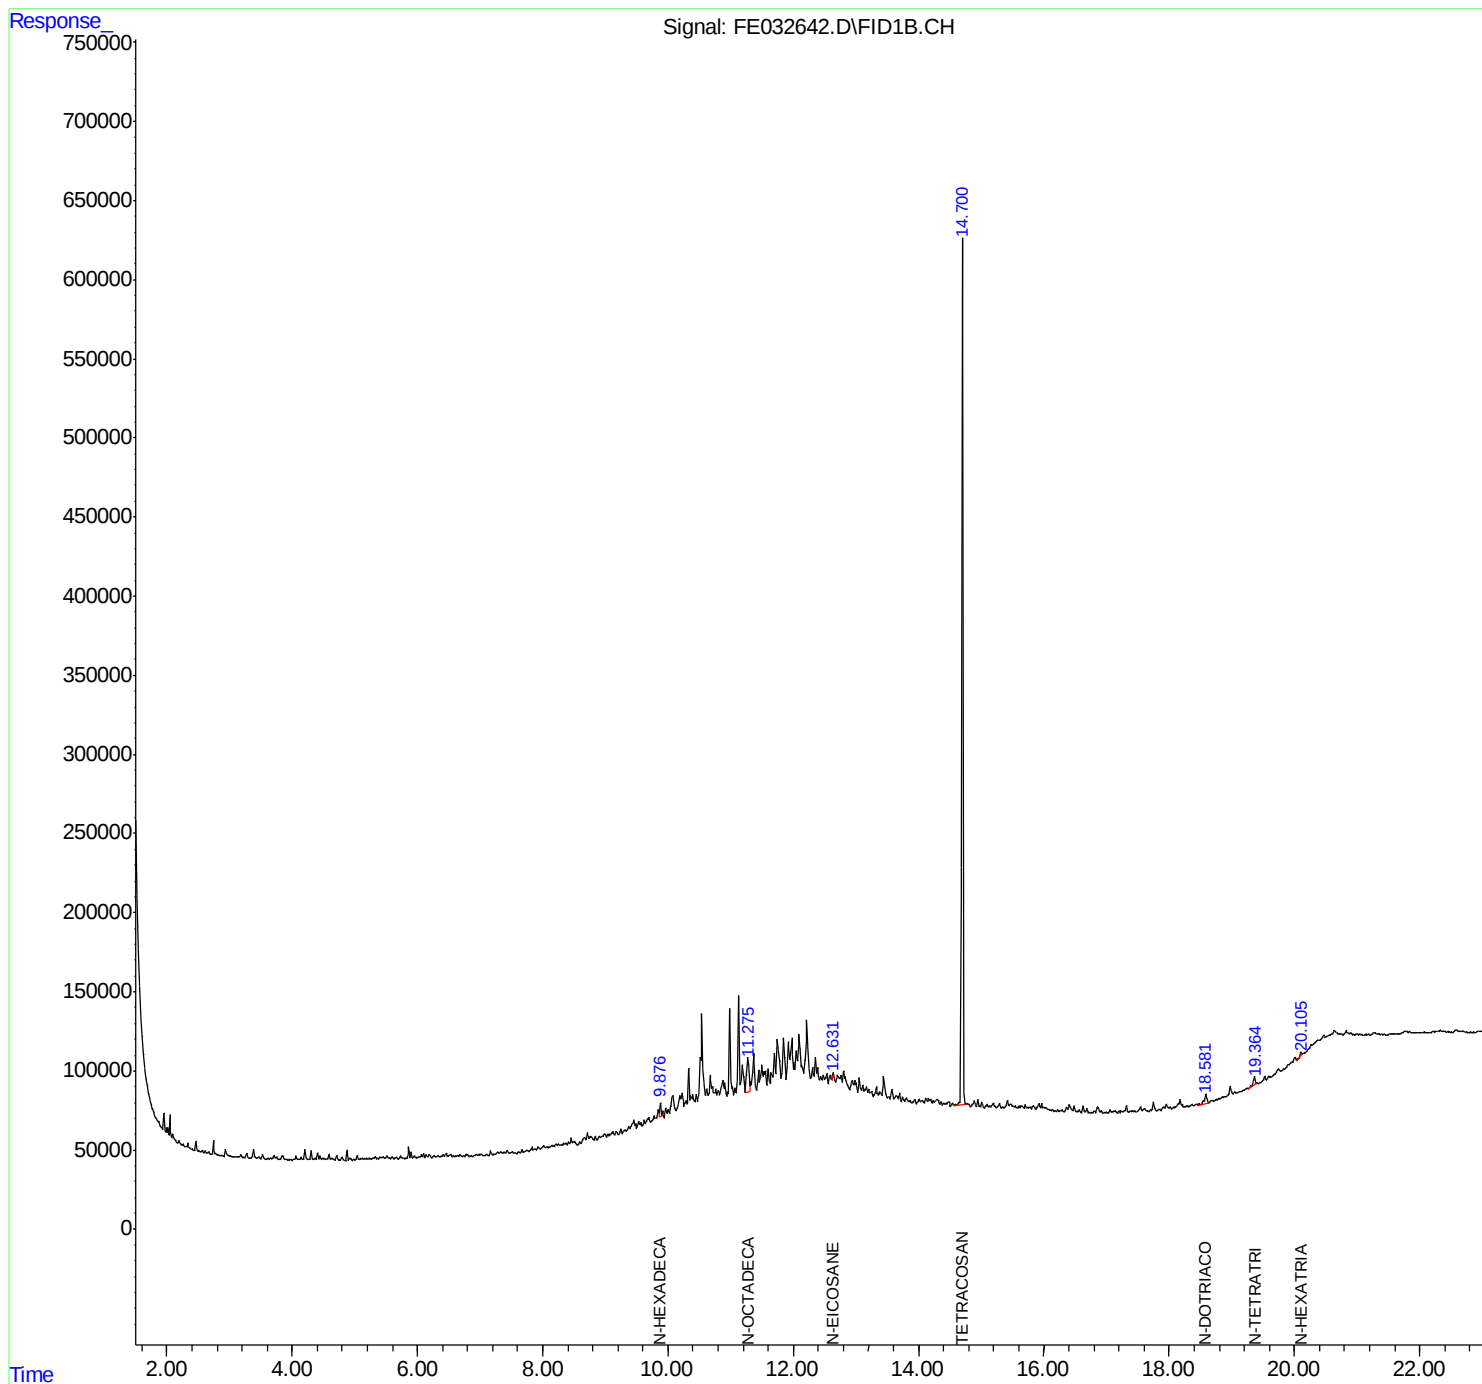


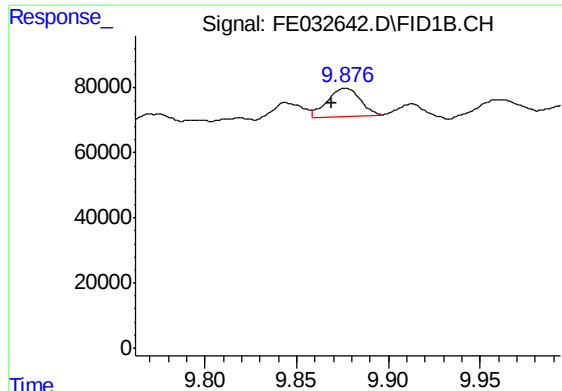

#5 N-HEXADECANE


R.T.: 9.876 min
Delta R.T.: 0.007 min
Response: 110138
Conc: 0.30 ug/ml

Instrument :
FID_E
ClientSampleId :
SIMW-07-20200827

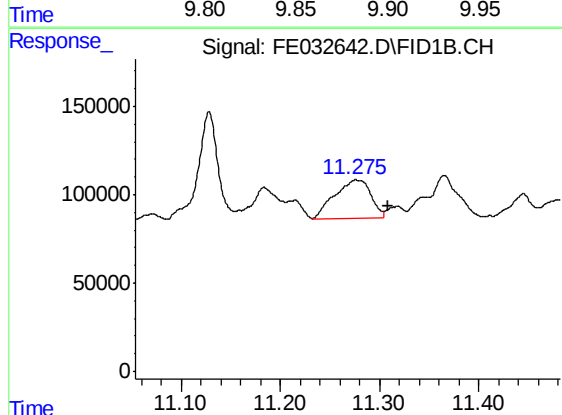


#6 N-OCTADECANE

R.T.: 11.276 min
Delta R.T.: -0.033 min
Response: 551105
Conc: 1.48 ug/ml

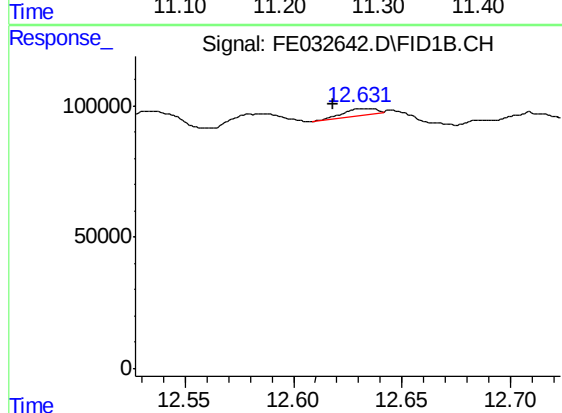


#7 N-EICOSANE

R.T.: 12.631 min
Delta R.T.: 0.013 min
Response: 24741
Conc: 0.07 ug/ml

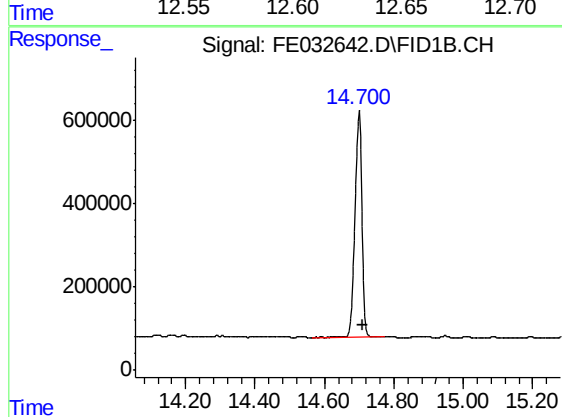

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.700 min
Delta R.T.: -0.011 min
Response: 7586162
Conc: 23.57 ug/ml

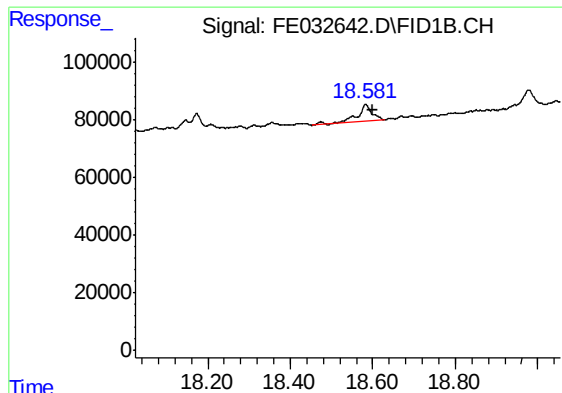

#14 N-DOTRIACONTANE


R.T.: 18.582 min
Delta R.T.: -0.019 min
Response: 150882
Conc: 0.43 ug/ml

Instrument :
FID_E
ClientSampleId :
SIMW-07-20200827

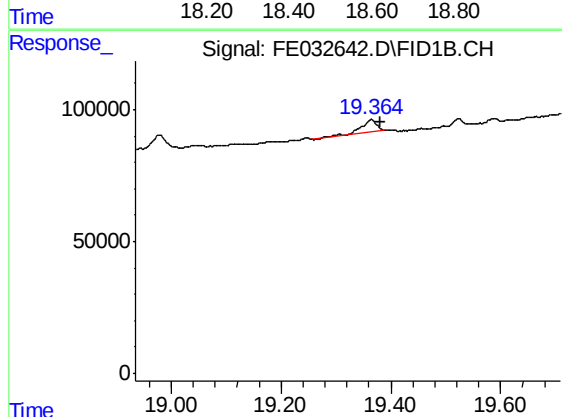

#15 N-TETRATRIACONTANE

R.T.: 19.365 min
Delta R.T.: -0.016 min
Response: 90194
Conc: 0.31 ug/ml

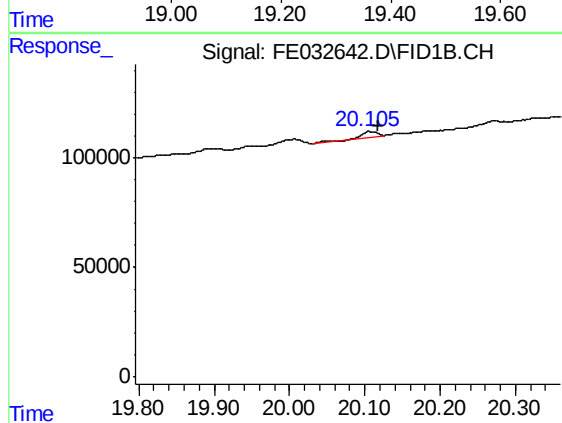

#16 N-HEXATRIACONTANE

R.T.: 20.105 min
Delta R.T.: -0.012 min
Response: 36646
Conc: 0.16 ug/ml