

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE083022\  
Data File : FE037304.D  
Signal(s) : FID1B.ch  
Acq On : 30 Aug 2022 10:09  
Operator : YP\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Aug 31 13:21:56 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE082922.M  
Quant Title :  
QLast Update : Mon Aug 29 16:06:19 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    |              | R.T.   | Response | Conc Units   |
|-----------------------------|--------------|--------|----------|--------------|
| -----                       |              |        |          |              |
| System Monitoring Compounds |              |        |          |              |
| Target Compounds            |              |        |          |              |
| 3)                          | N-DODECANE   | 6.472  | 2472874  | 15.198 ug/ml |
| 12)                         | N-OCTACOSANE | 16.875 | 2337576  | 15.172 ug/ml |
| -----                       |              |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE083022\  
Data File : FE037304.D  
Signal(s) : FID1B.ch  
Acq On : 30 Aug 2022 10:09  
Operator : YP\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Aug 31 13:21:56 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE082922.M  
Quant Title :  
QLast Update : Mon Aug 29 16:06:19 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

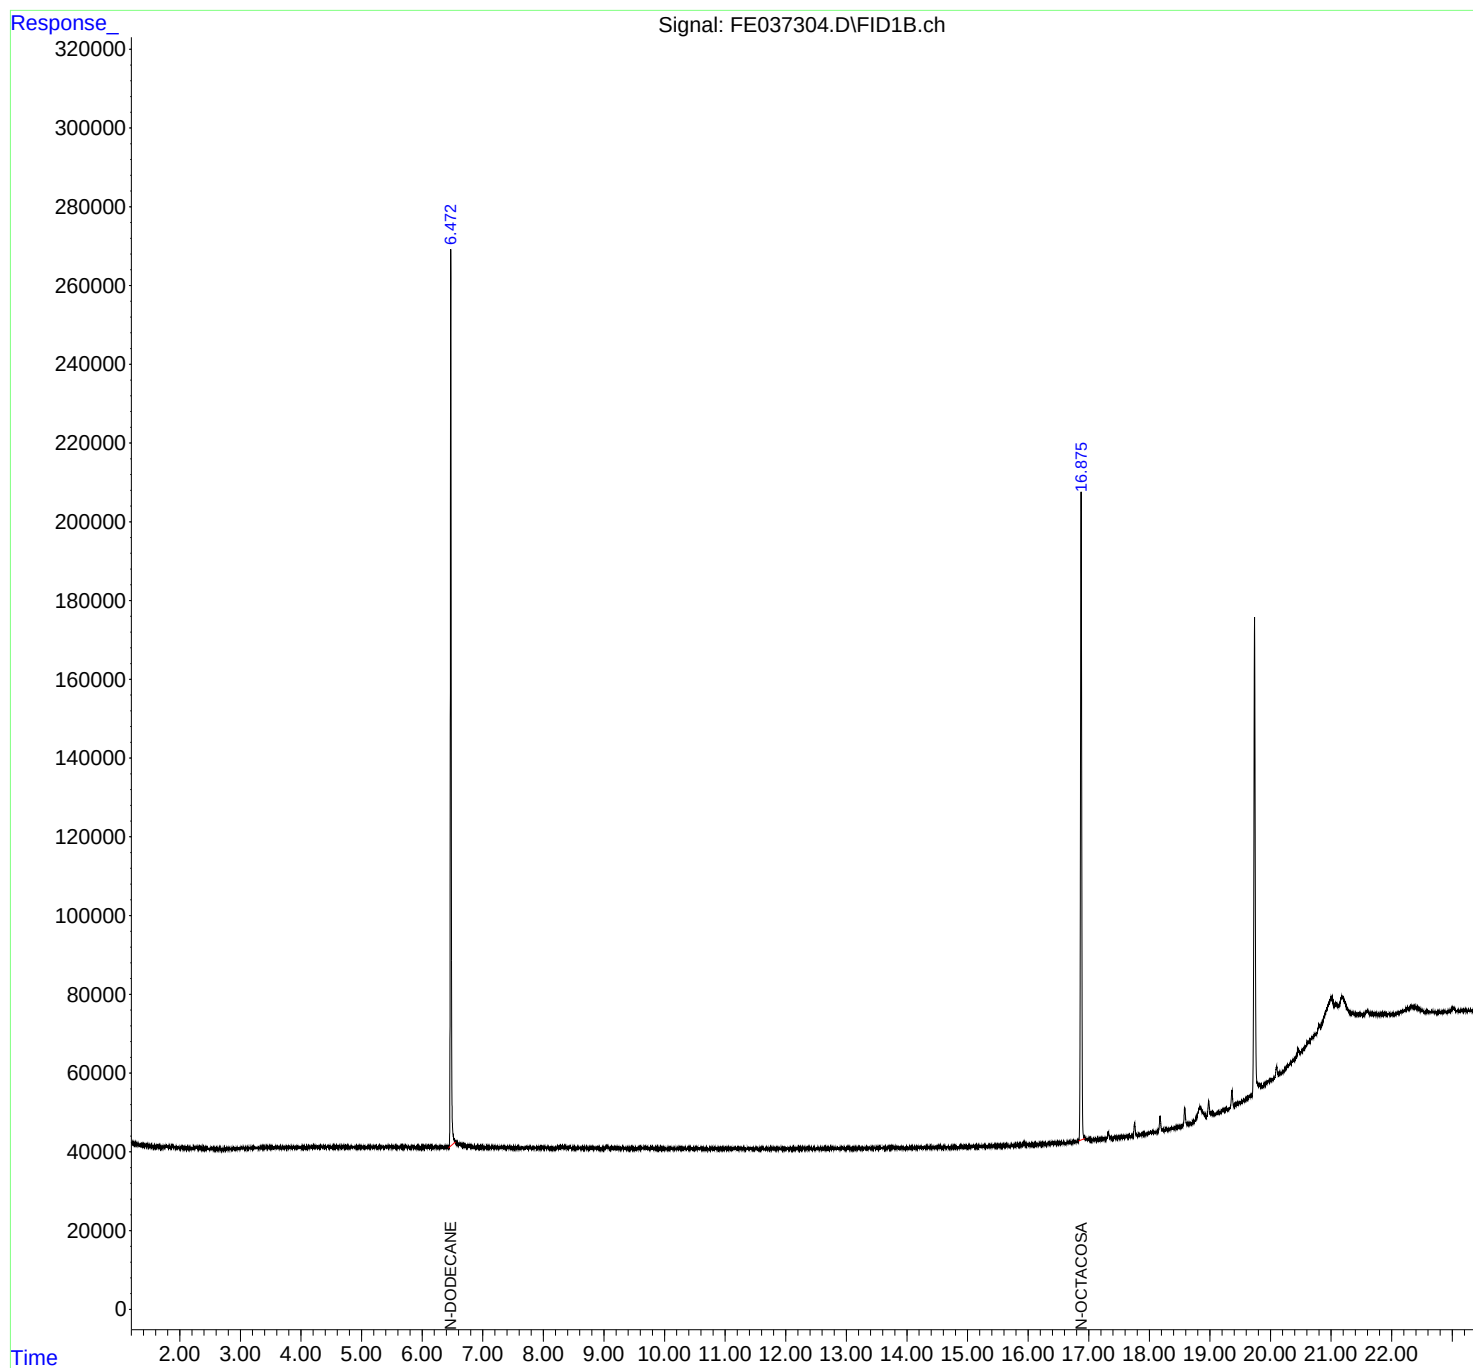


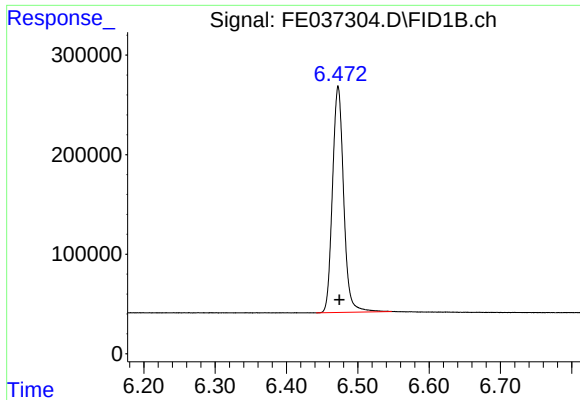

#3 N-DODECANE


R.T.: 6.472 min  
Delta R.T.: -0.002 min  
Response: 2472874  
Conc: 15.20 ug/ml

Instrument :  
FID\_E  
ClientSampleId :

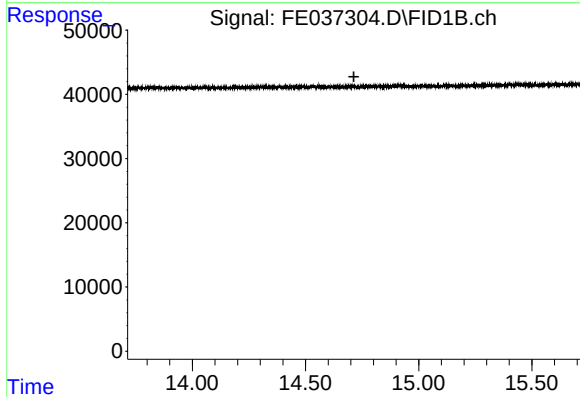

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 14.714 min  
Response: 0  
Conc: N.D.

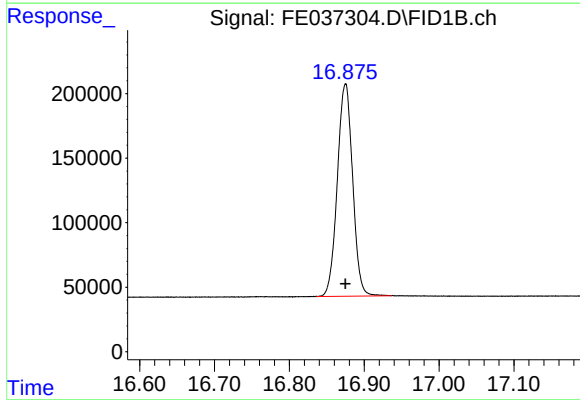

#12 N-OCTACOSANE

R.T.: 16.875 min  
Delta R.T.: 0.000 min  
Response: 2337576  
Conc: 15.17 ug/ml