

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083022\
Data File : FE037317.D
Signal(s) : FID1B.ch
Acq On : 30 Aug 2022 17:30
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 31 13:24:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE082922.M
Quant Title :
QLast Update : Mon Aug 29 16:06:19 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.471	2406242	14.788 ug/ml
12) N-OCTACOSANE	16.873	2284935	14.831 ug/ml
14) N-DOTRIACONTANE	18.582	124504	0.832 ug/ml
15) N-TETRATRIACONTANE	19.362	112078	0.771 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083022\
Data File : FE037317.D
Signal(s) : FID1B.ch
Acq On : 30 Aug 2022 17:30
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 31 13:24:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE082922.M
Quant Title :
QLast Update : Mon Aug 29 16:06:19 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

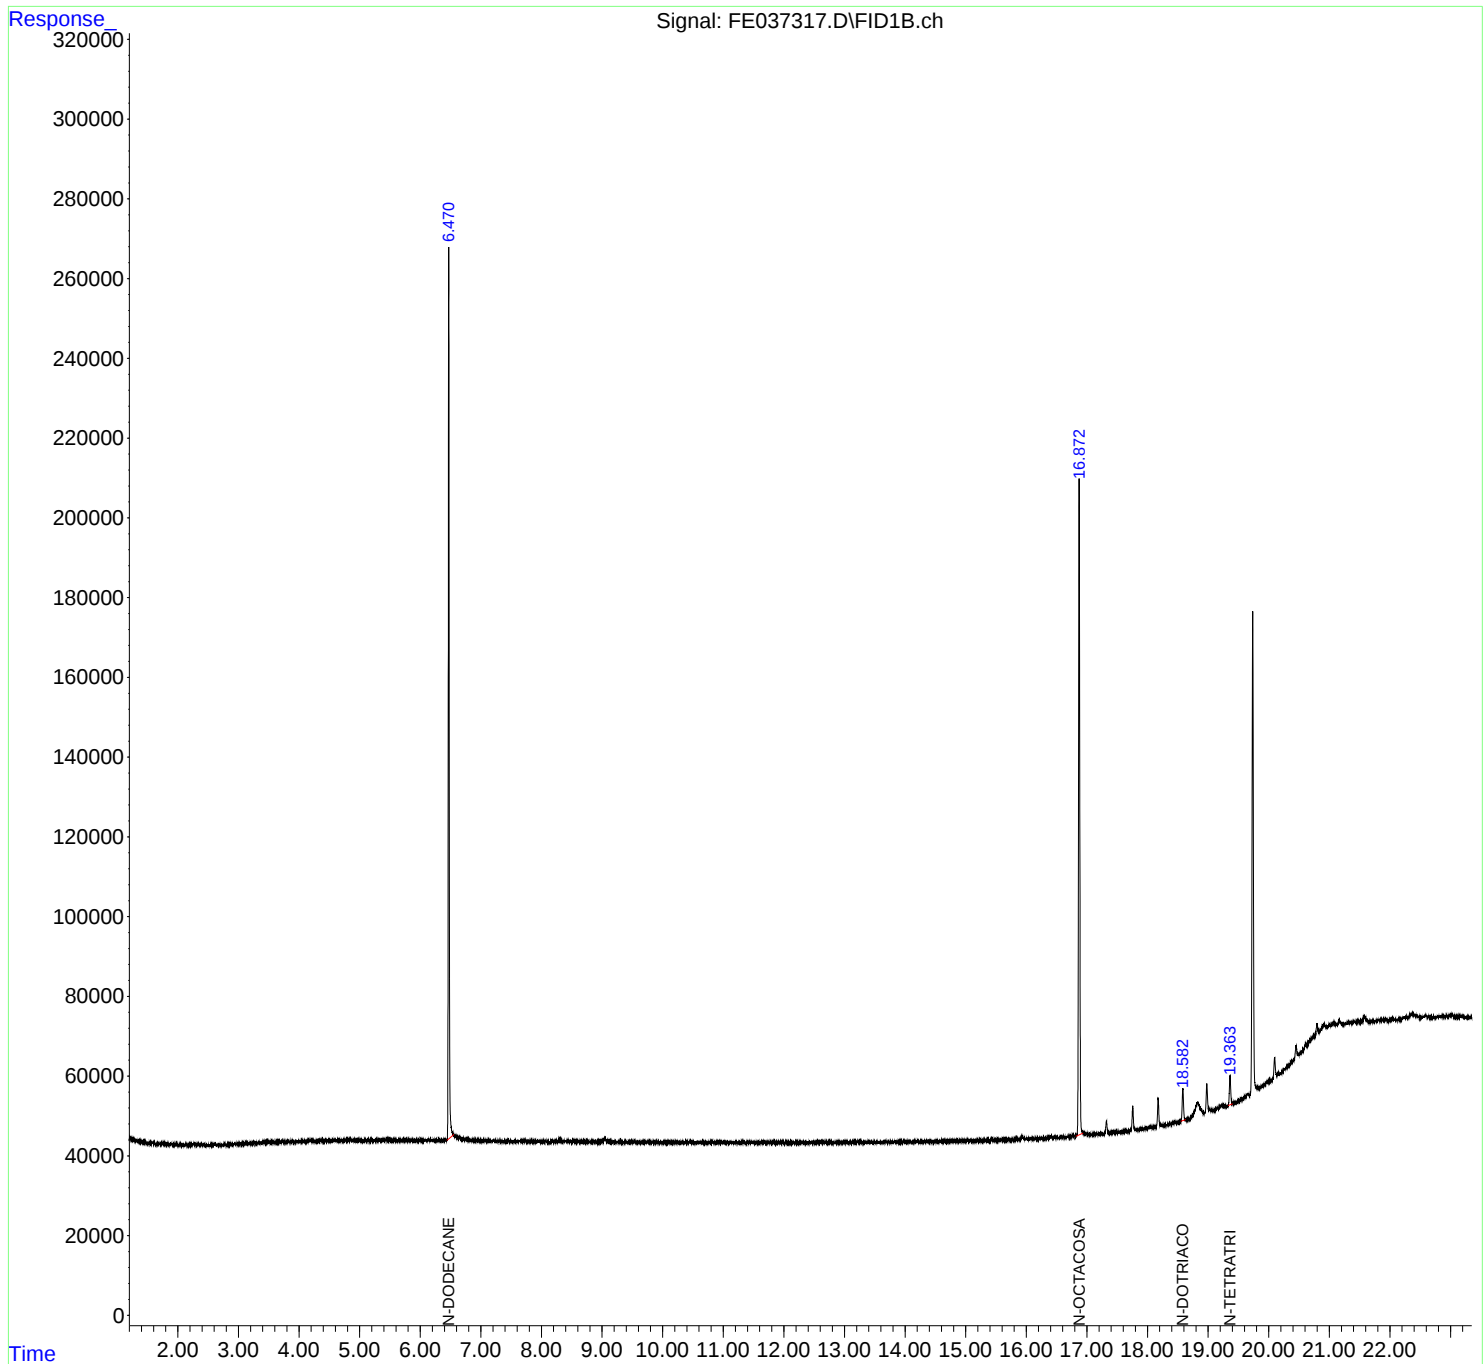


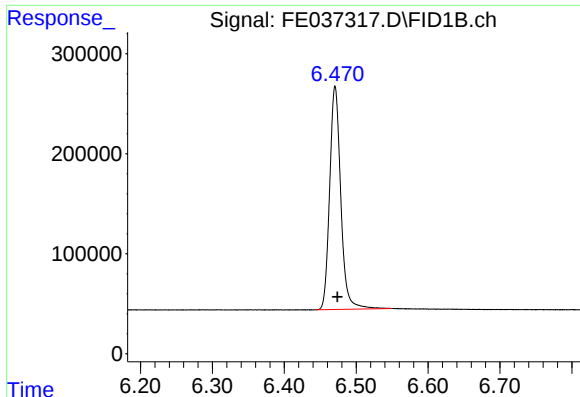

#3 N-DODECANE


R.T.: 6.471 min
Delta R.T.: -0.003 min
Response: 2406242
Conc: 14.79 ug/ml

Instrument :
FID_E
ClientSampleId :

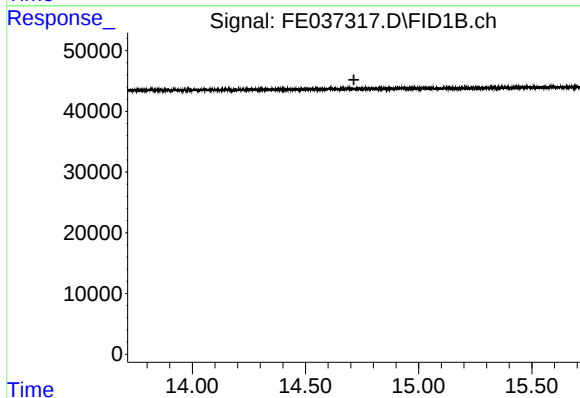


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.714 min
Response: 0
Conc: N.D.

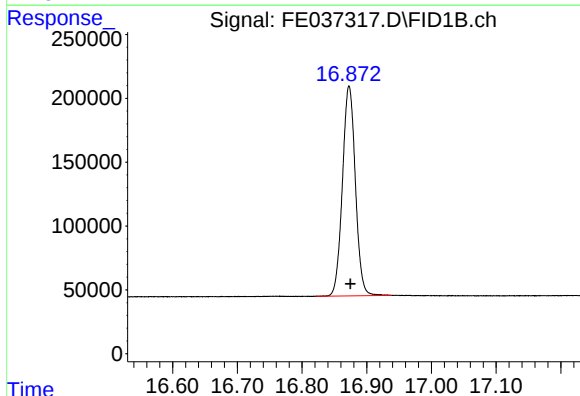


#12 N-OCTACOSANE

R.T.: 16.873 min
Delta R.T.: -0.002 min
Response: 2284935
Conc: 14.83 ug/ml

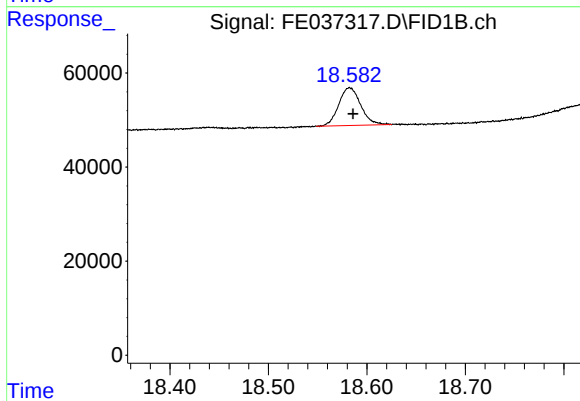

#14 N-DOTRIACONTANE

R.T.: 18.582 min
Delta R.T.: -0.004 min
Response: 124504
Conc: 0.83 ug/ml

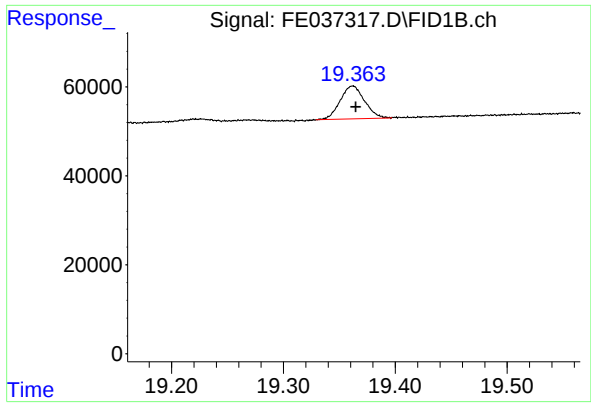

#15 N-TETRATRIACONTANE

R.T.: 19.362 min
Delta R.T.: -0.003 min
Response: 112078
Conc: 0.77 ug/ml

Instrument :
FID_E
ClientSampleId :