

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083022\
 Data File : FE037318.D
 Signal(s) : FID1B.ch
 Acq On : 30 Aug 2022 18:02
 Operator : YP\AJ
 Sample : PB146676BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 31 13:24:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE082922.M
 Quant Title :
 QLast Update : Mon Aug 29 16:06:19 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.712	3155446	22.025 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.756	97210	0.640 ug/ml
14) N-DOTRIACONTANE	18.581	126797	0.848 ug/ml
15) N-TETRATRIACONTANE	19.361	94254	0.648 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083022\
Data File : FE037318.D
Signal(s) : FID1B.ch
Acq On : 30 Aug 2022 18:02
Operator : YP\AJ
Sample : PB146676BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 31 13:24:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE082922.M
Quant Title :
QLast Update : Mon Aug 29 16:06:19 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

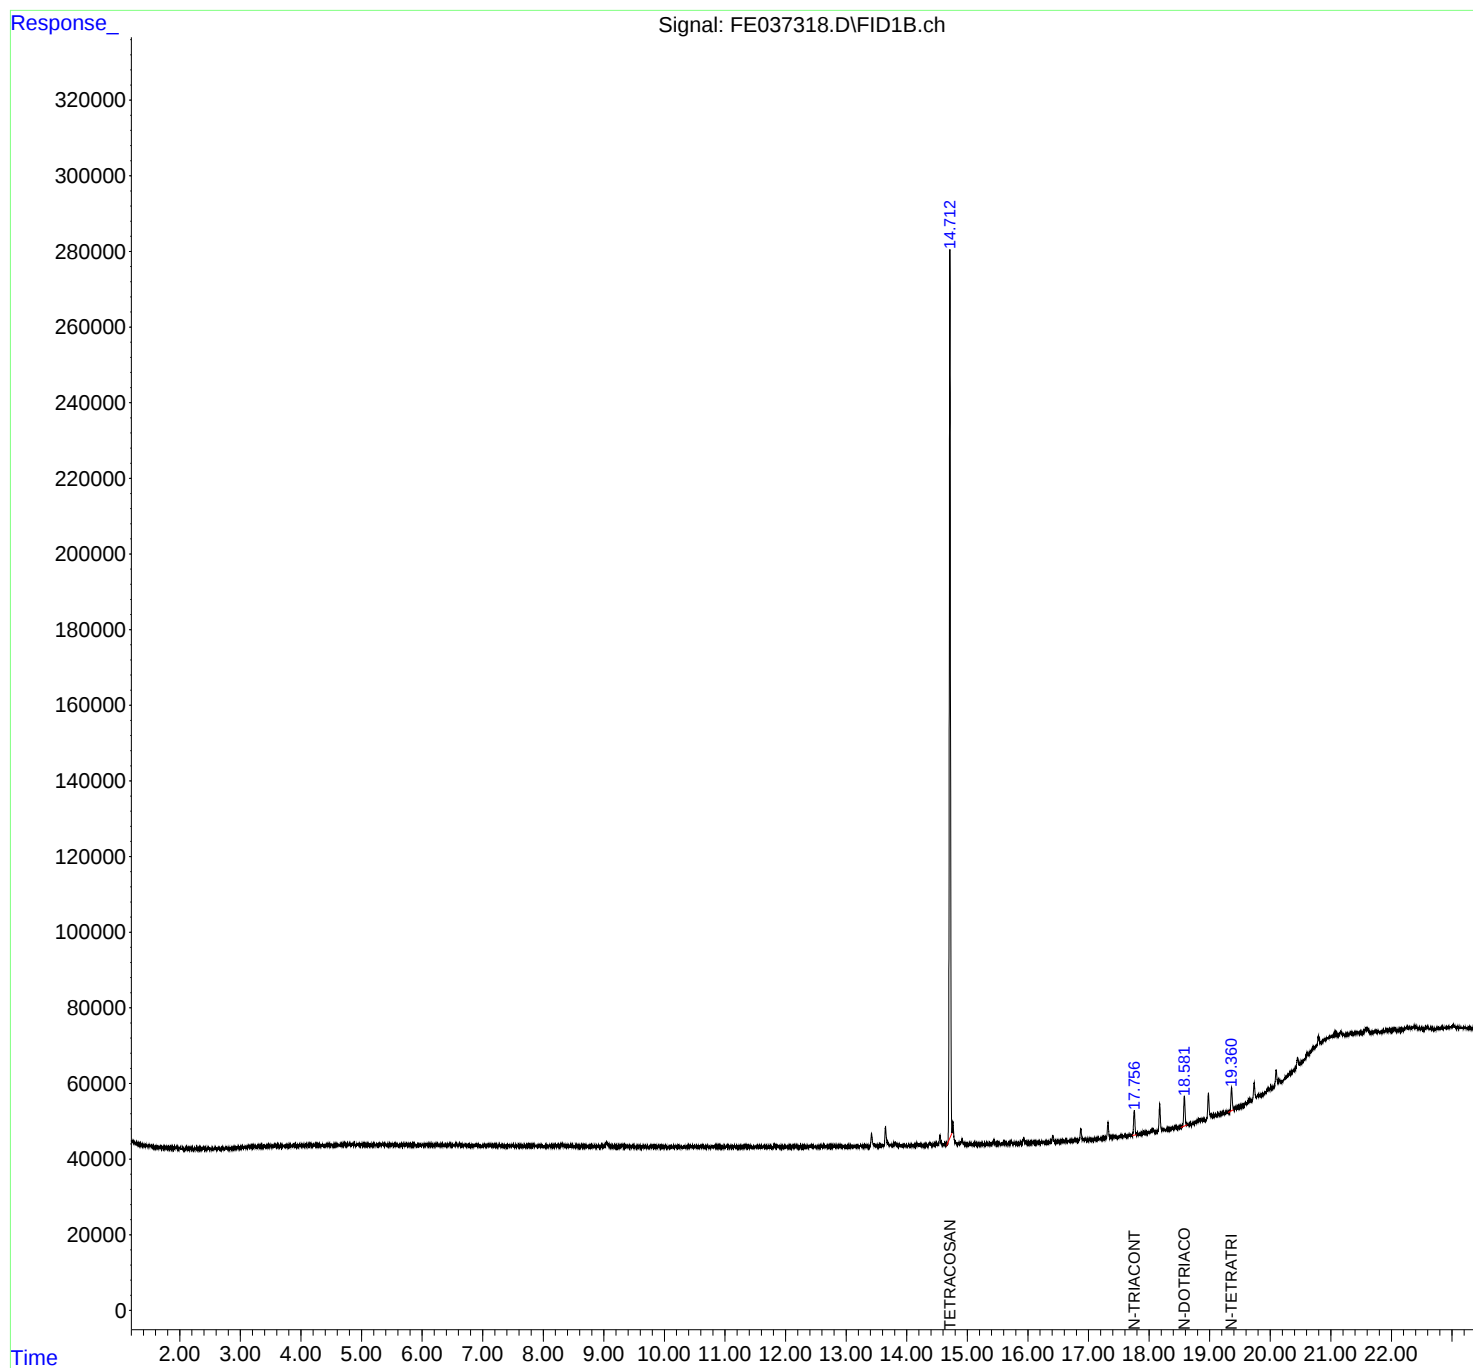


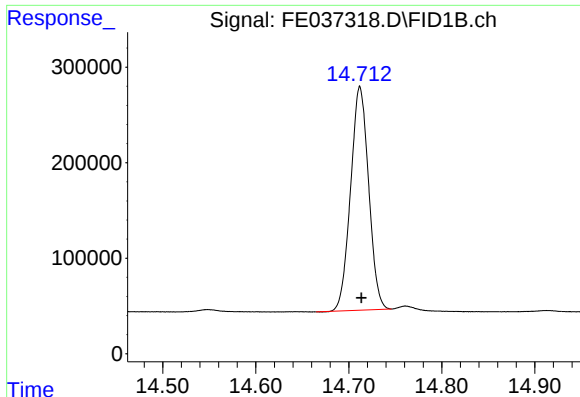

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.712 min
Delta R.T.: -0.002 min
Response: 3155446
Conc: 22.03 ug/ml

Instrument :
FID_E
ClientSampleId :

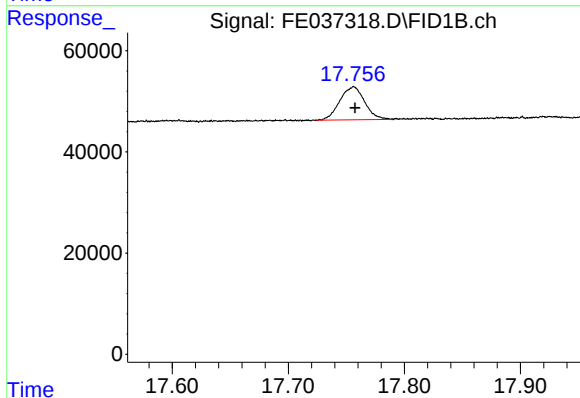


#13 N-TRIACONTANE

R.T.: 17.756 min
Delta R.T.: -0.001 min
Response: 97210
Conc: 0.64 ug/ml

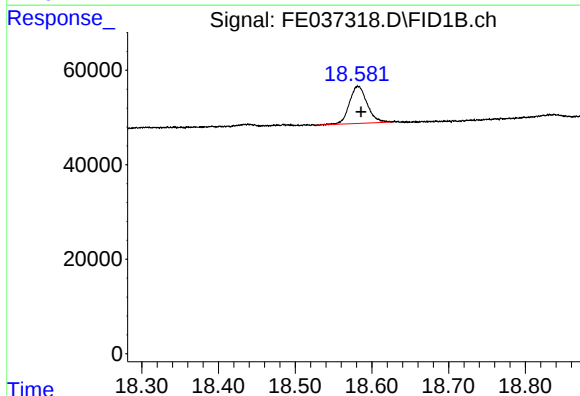

#14 N-DOTRIACONTANE

R.T.: 18.581 min
Delta R.T.: -0.005 min
Response: 126797
Conc: 0.85 ug/ml

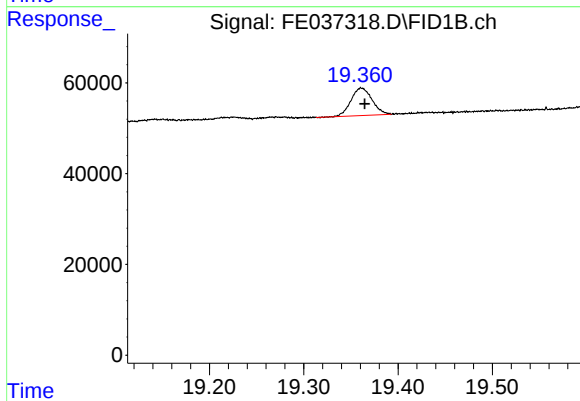

#15 N-TETRATRIACONTANE

R.T.: 19.361 min
Delta R.T.: -0.004 min
Response: 94254
Conc: 0.65 ug/ml