

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083022\
Data File : FE037319.D
Signal(s) : FID1B.ch
Acq On : 30 Aug 2022 18:33
Operator : YP\AJ
Sample : PB146681BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 31 13:24:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE082922.M
Quant Title :
QLast Update : Mon Aug 29 16:06:19 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.712	2959284	20.656 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.583	97980	0.655 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083022\
Data File : FE037319.D
Signal(s) : FID1B.ch
Acq On : 30 Aug 2022 18:33
Operator : YP\AJ
Sample : PB146681BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 31 13:24:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE082922.M
Quant Title :
QLast Update : Mon Aug 29 16:06:19 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

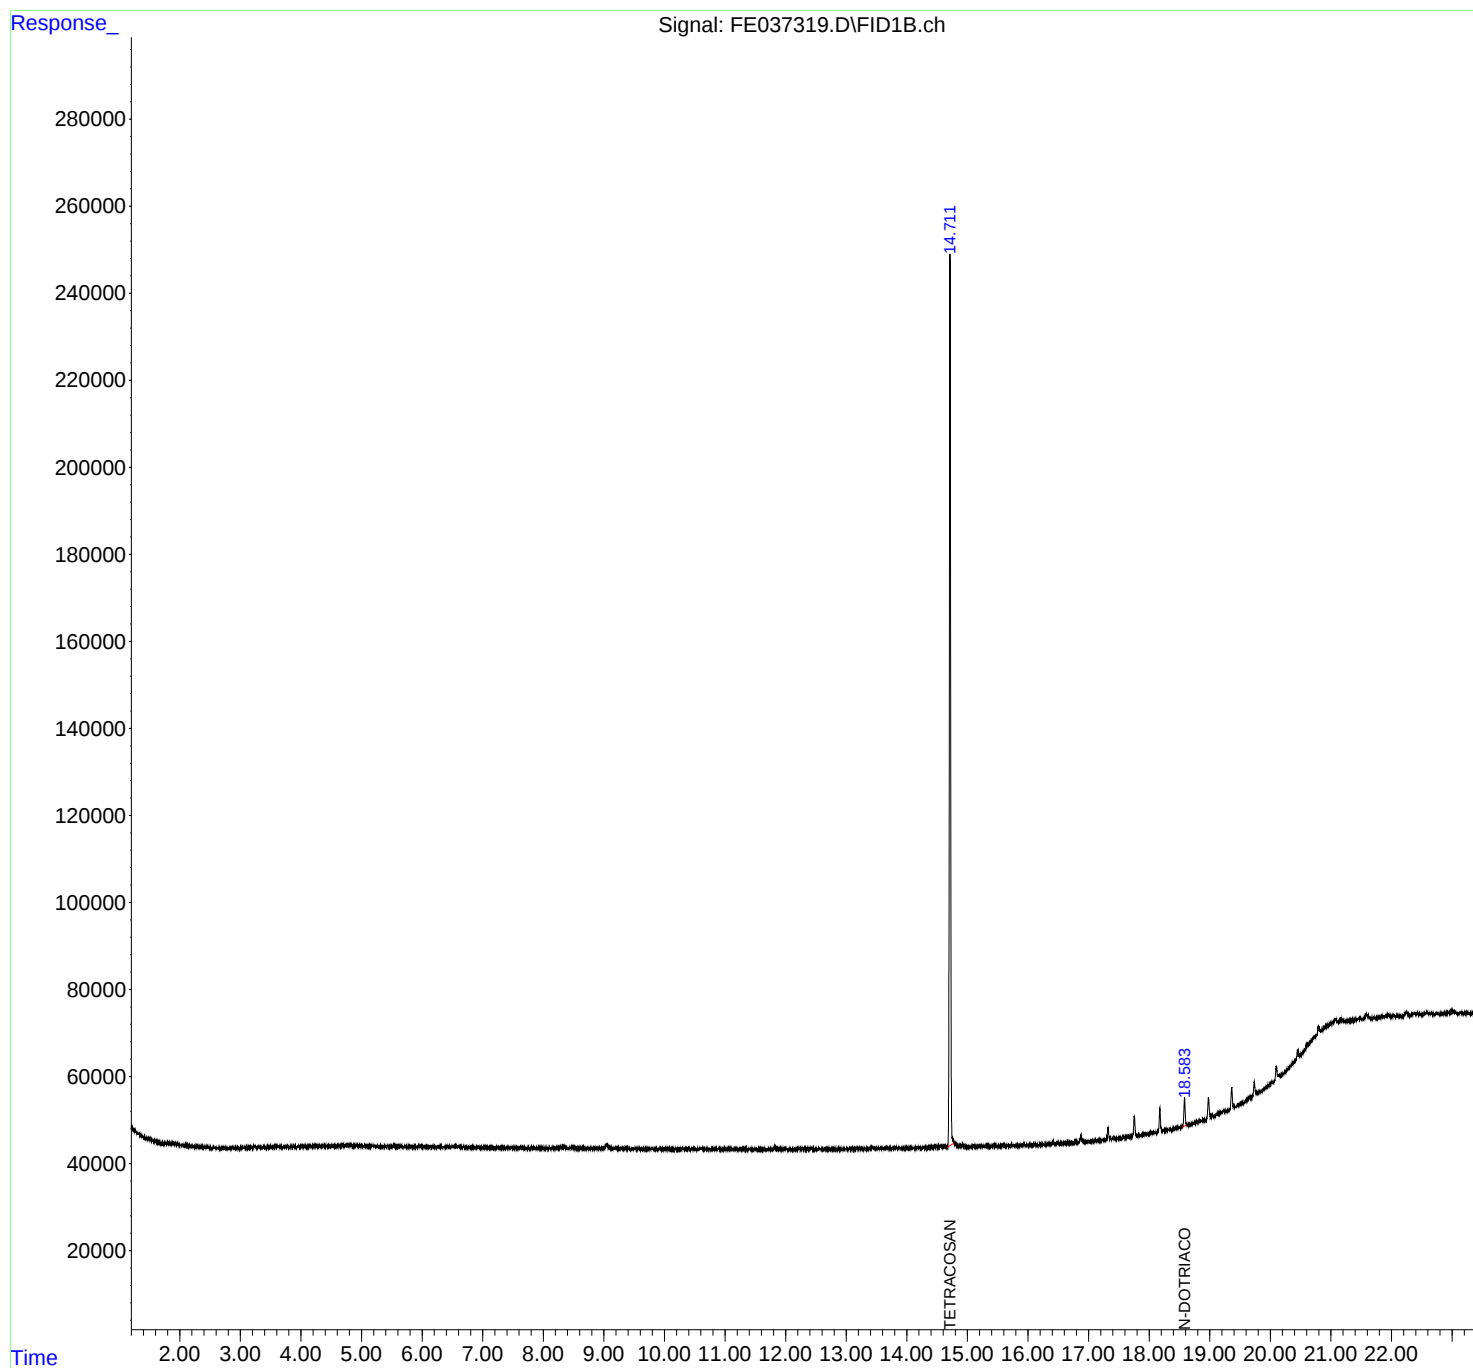


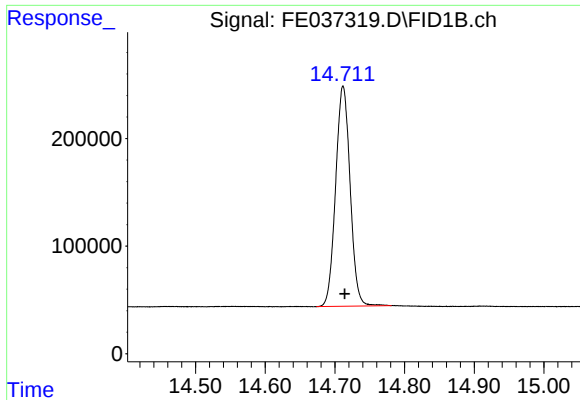

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.712 min
Delta R.T.: -0.002 min
Response: 2959284
Conc: 20.66 ug/ml

Instrument :
FID_E
ClientSampleId :

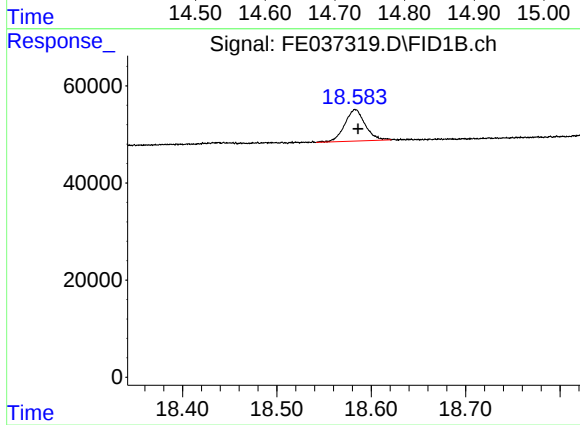

#14 N-DOTRIACONTANE

R.T.: 18.583 min
Delta R.T.: -0.003 min
Response: 97980
Conc: 0.66 ug/ml