

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083022\
 Data File : FE037321.D
 Signal(s) : FID1B.ch
 Acq On : 30 Aug 2022 19:35
 Operator : YP\AJ
 Sample : N3980-04
 Misc : 2.5 PPM SOIL LOD
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 31 13:25:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE082922.M
 Quant Title :
 QLast Update : Mon Aug 29 16:06:19 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.711	2036929	14.218 ug/ml
Target Compounds			
1) N-OCTANE	1.803	260901	1.717 ug/ml
2) N-DECANE	4.302	211287	1.341 ug/ml
3) N-DODECANE	6.473	195755	1.203 ug/ml
4) N-TETRADECANE	8.291	223868	1.335 ug/ml
5) N-HEXADECANE	9.889	220367	1.294 ug/ml
6) N-OCTADECANE	11.323	233841	1.361 ug/ml
7) N-EICOSANE	12.624	243545	1.431 ug/ml
8) N-DOCOSANE	13.816	268914	1.624 ug/ml
10) N-TETRACOSANE	14.912	282069	1.722 ug/ml
11) N-HEXACOSANE	15.927	264415	1.664 ug/ml
12) N-OCTACOSANE	16.872	263093	1.708 ug/ml
13) N-TRIACONTANE	17.755	271633	1.789 ug/ml
14) N-DOTRIACONTANE	18.581	260074	1.739 ug/ml
15) N-TETRATRIACONTANE	19.361	219512	1.509 ug/ml
16) N-HEXATRIACONTANE	20.097	186977	1.368 ug/ml
17) N-OCTATRIACONTANE	20.795	185925	1.395 ug/ml
18) N-TETRACONTANE	21.574	182285	1.324 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083022\
Data File : FE037321.D
Signal(s) : FID1B.ch
Acq On : 30 Aug 2022 19:35
Operator : YP\AJ
Sample : N3980-04
Misc : 2.5 PPM SOIL LOD
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 31 13:25:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE082922.M
Quant Title :
QLast Update : Mon Aug 29 16:06:19 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

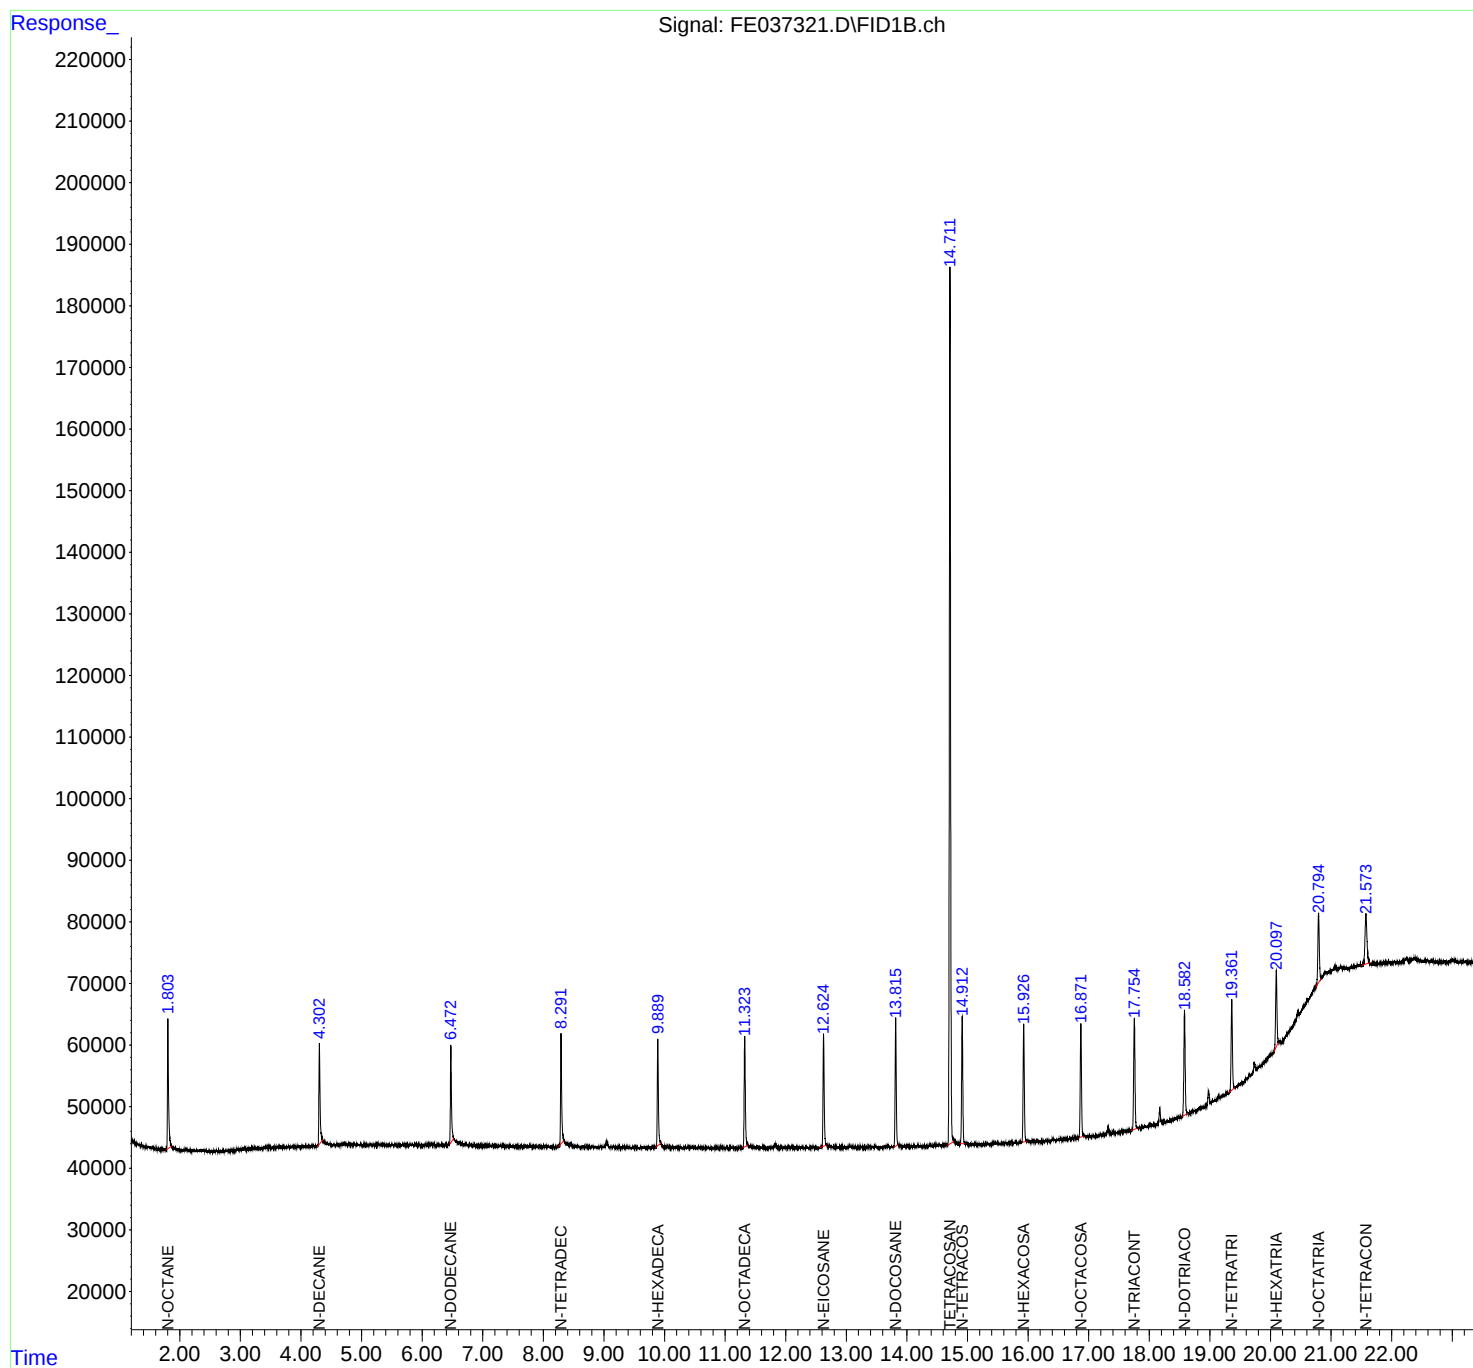


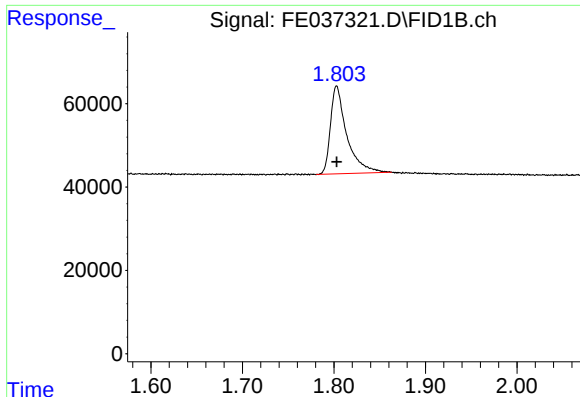

#1 N-OCTANE


R.T.: 1.803 min
Delta R.T.: 0.000 min
Response: 260901
Conc: 1.72 ug/ml

Instrument :
FID_E
ClientSampleId :

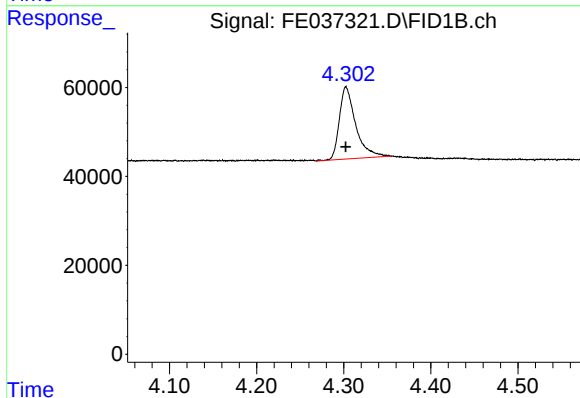


#2 N-DECANE

R.T.: 4.302 min
Delta R.T.: 0.000 min
Response: 211287
Conc: 1.34 ug/ml

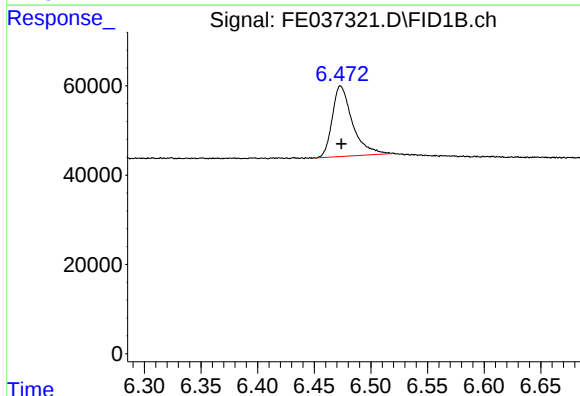


#3 N-DODECANE

R.T.: 6.473 min
Delta R.T.: -0.001 min
Response: 195755
Conc: 1.20 ug/ml

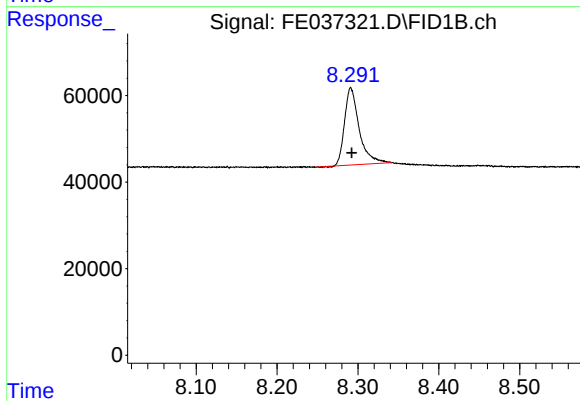

#4 N-TETRADECANE


R.T.: 8.291 min
Delta R.T.: -0.001 min
Response: 223868
Conc: 1.34 ug/ml

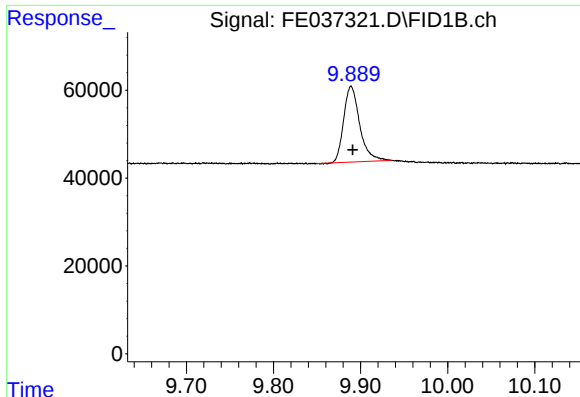

#5 N-HEXADECANE


R.T.: 9.889 min
Delta R.T.: -0.002 min
Response: 220367
Conc: 1.29 ug/ml

Instrument :
FID_E
ClientSampleId :

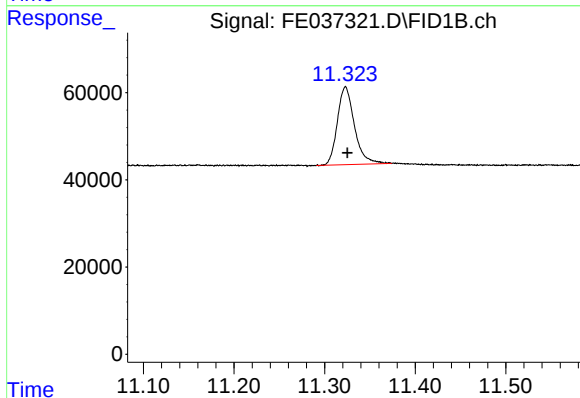


#6 N-OCTADECANE

R.T.: 11.323 min
Delta R.T.: -0.002 min
Response: 233841
Conc: 1.36 ug/ml

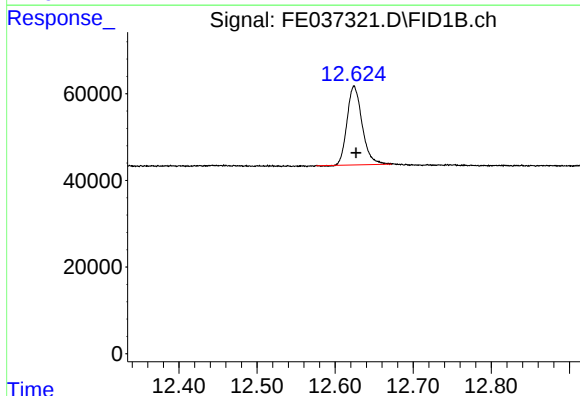


#7 N-EICOSANE

R.T.: 12.624 min
Delta R.T.: -0.003 min
Response: 243545
Conc: 1.43 ug/ml

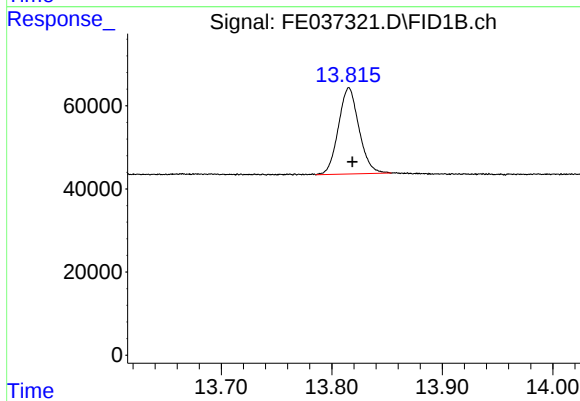

#8 N-DOCOSANE


R.T.: 13.816 min
Delta R.T.: -0.003 min
Response: 268914
Conc: 1.62 ug/ml

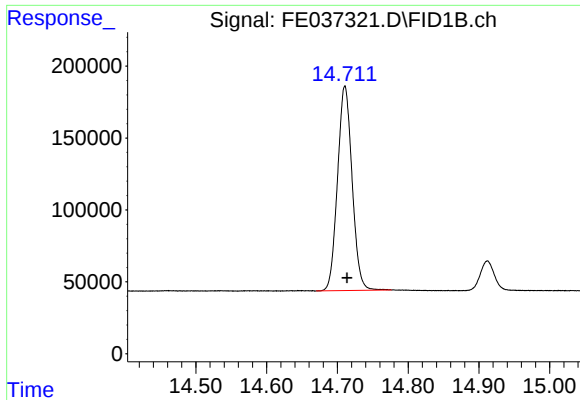

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.711 min
Delta R.T.: -0.003 min
Response: 2036929
Conc: 14.22 ug/ml

Instrument :
FID_E
ClientSampleId :

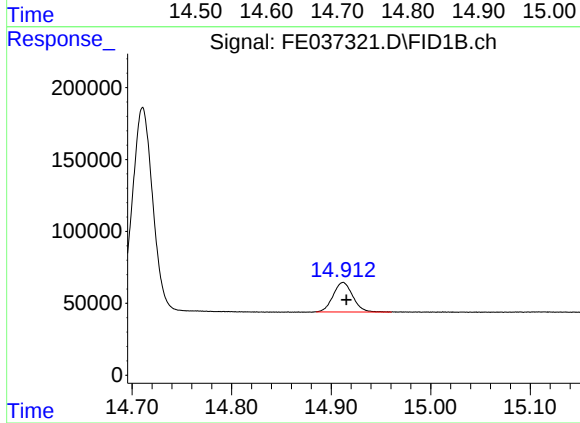


#10 N-TETRACOSANE

R.T.: 14.912 min
Delta R.T.: -0.003 min
Response: 282069
Conc: 1.72 ug/ml

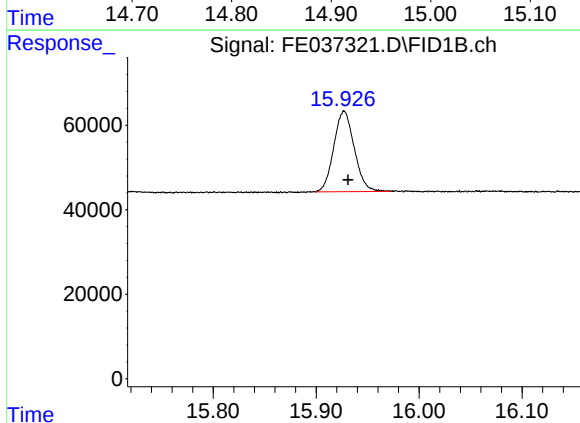


#11 N-HEXACOSANE

R.T.: 15.927 min
Delta R.T.: -0.004 min
Response: 264415
Conc: 1.66 ug/ml

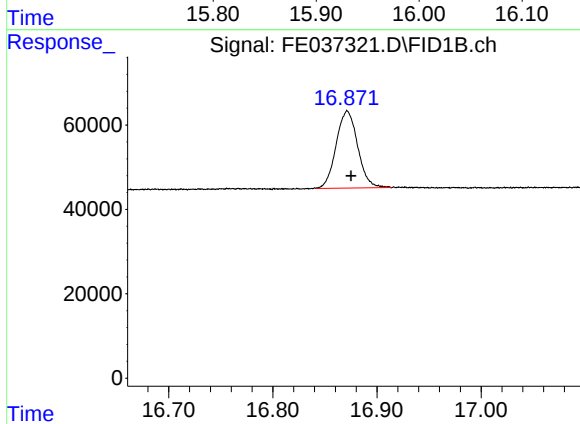

#12 N-OCTACOSANE


R.T.: 16.872 min
Delta R.T.: -0.004 min
Response: 263093
Conc: 1.71 ug/ml

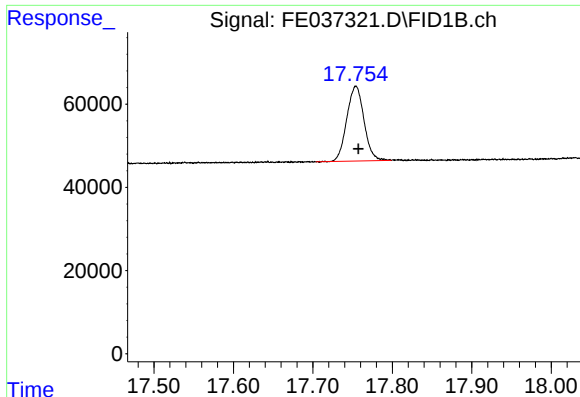

#13 N-TRIACONTANE


R.T.: 17.755 min
Delta R.T.: -0.003 min
Response: 271633
Conc: 1.79 ug/ml

Instrument :
FID_E
ClientSampleId :

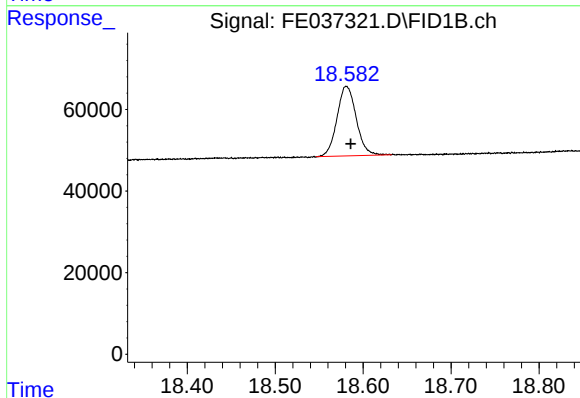


#14 N-DOTRIACONTANE

R.T.: 18.581 min
Delta R.T.: -0.005 min
Response: 260074
Conc: 1.74 ug/ml

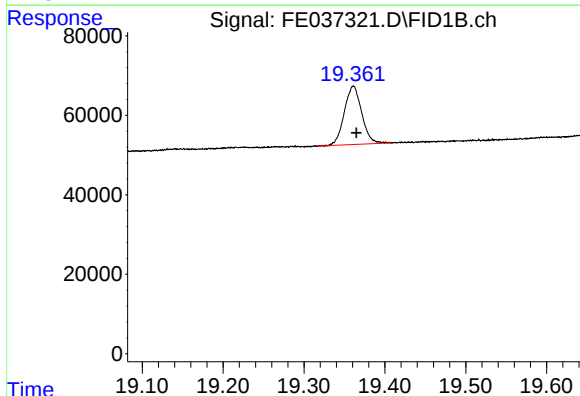


#15 N-TETRATRIACONTANE

R.T.: 19.361 min
Delta R.T.: -0.004 min
Response: 219512
Conc: 1.51 ug/ml

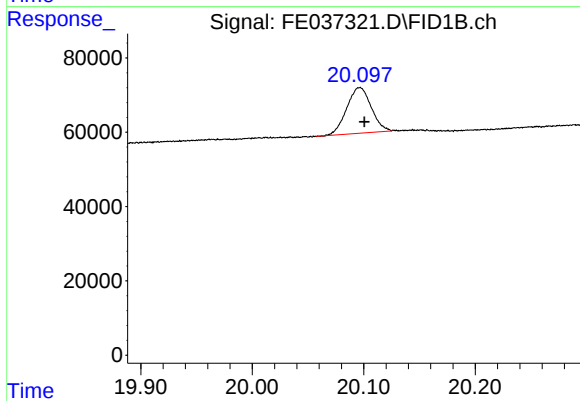

#16 N-HEXATRIACONTANE


R.T.: 20.097 min
Delta R.T.: -0.003 min
Response: 186977
Conc: 1.37 ug/ml

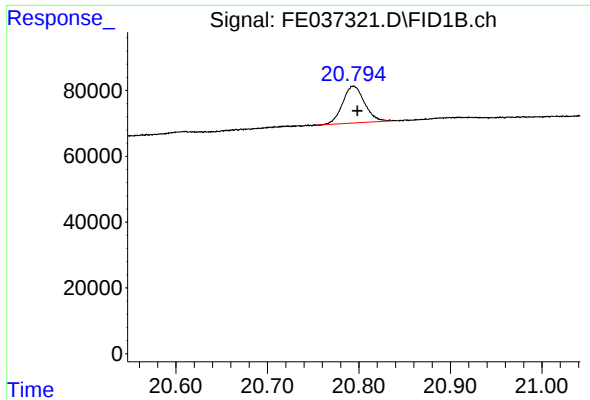

#17 N-OCTATRIACONTANE

R.T.: 20.795 min
Delta R.T.: -0.004 min
Response: 185925
Conc: 1.40 ug/ml

Instrument :
FID_E
ClientSampleId :

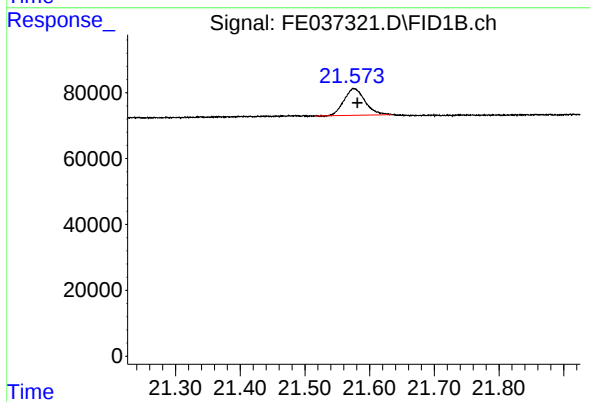

#18 N-TETRACONTANE

R.T.: 21.574 min
Delta R.T.: -0.007 min
Response: 182285
Conc: 1.32 ug/ml