

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083022\
Data File : FE037315.D
Signal(s) : FID1B.ch
Acq On : 30 Aug 2022 16:28
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Aug 31 13:24:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE082922.M
Quant Title :
QLast Update : Mon Aug 29 16:06:19 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.712	2325911	16.235 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083022\
Data File : FE037315.D
Signal(s) : FID1B.ch
Acq On : 30 Aug 2022 16:28
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Aug 31 13:24:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE082922.M
Quant Title :
QLast Update : Mon Aug 29 16:06:19 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

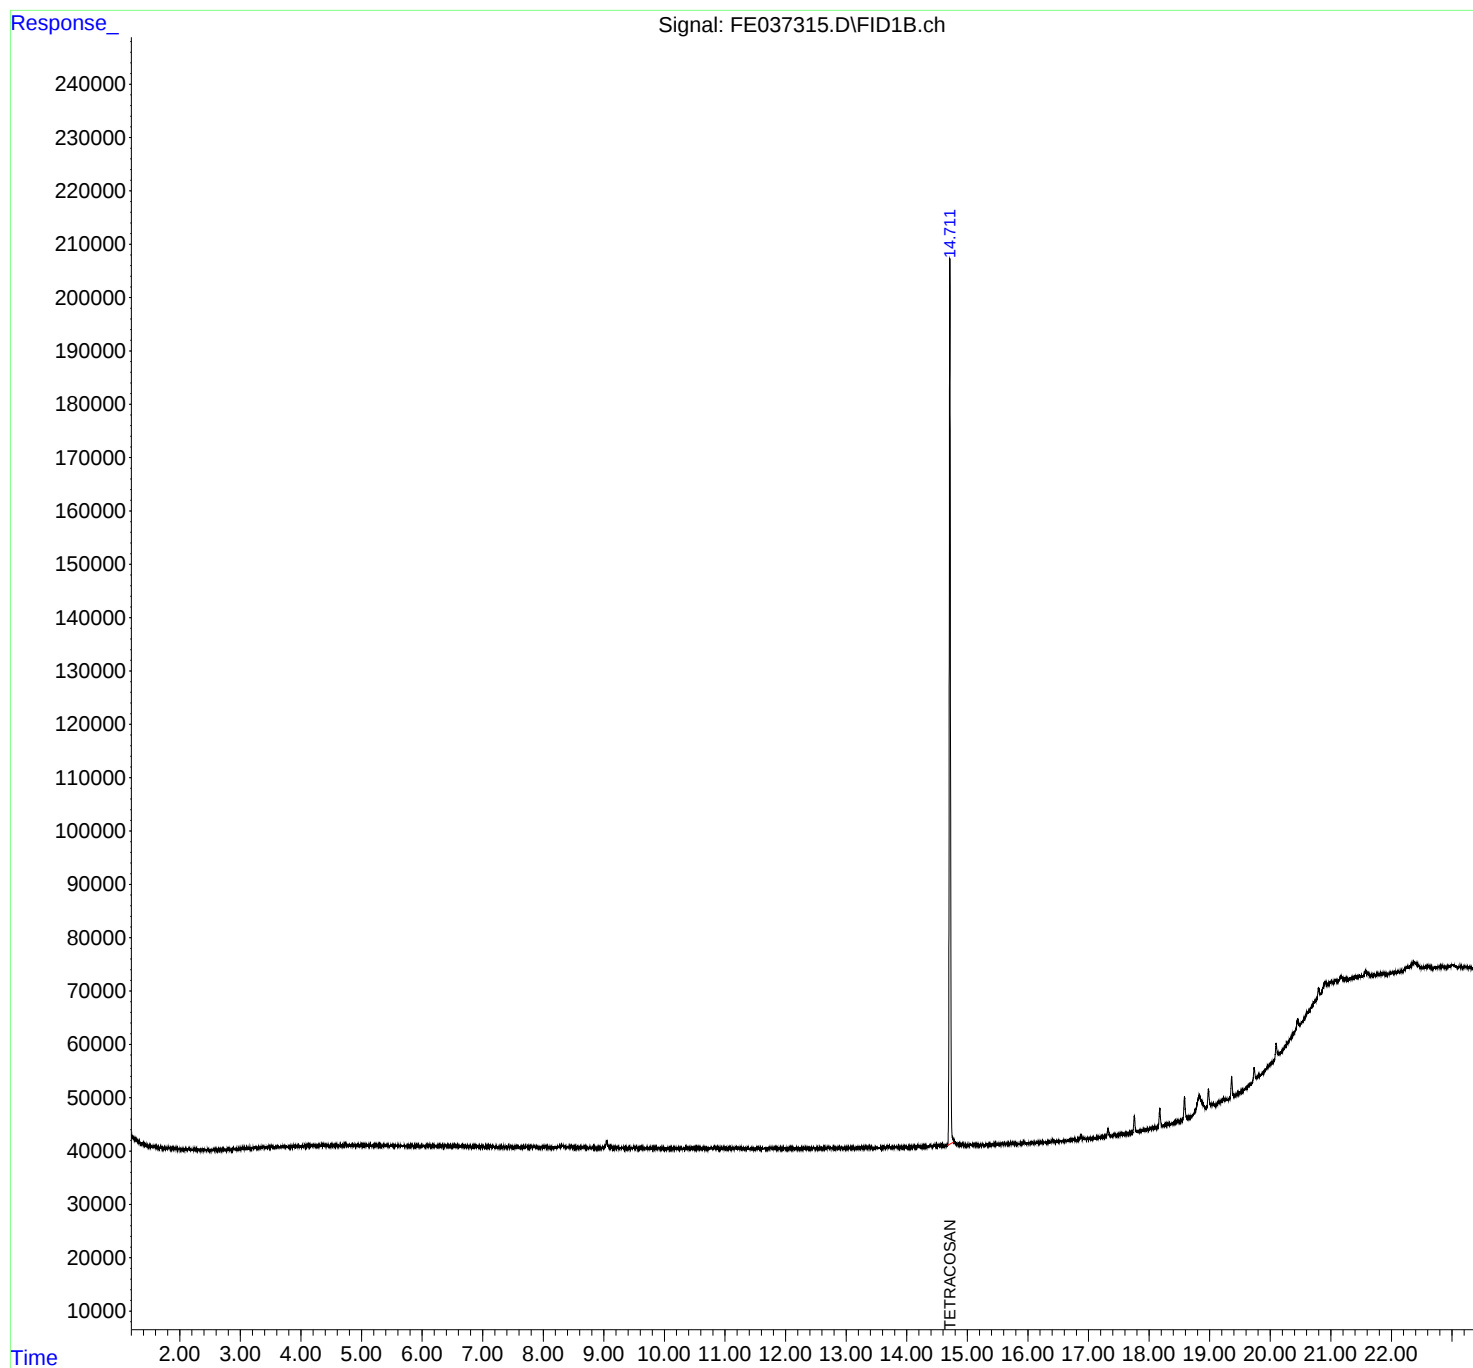

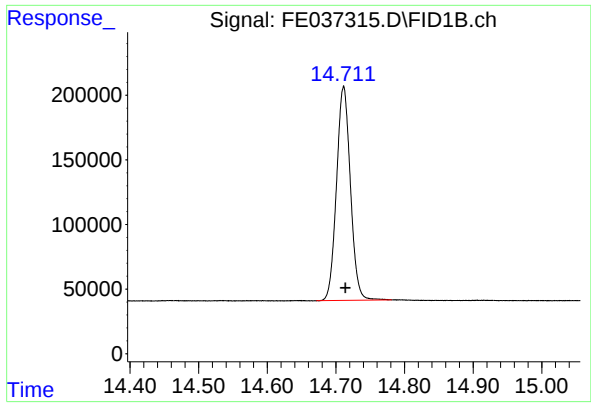

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.712 min
Delta R.T.: -0.002 min
Response: 2325911
Conc: 16.24 ug/ml

Instrument :
FID_E
ClientSampleId :
I.BLK