

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083022AL\
 Data File : FE037338.D
 Signal(s) : FID1B.ch
 Acq On : 31 Aug 2022 04:52
 Operator : YP\AJ
 Sample : N4424-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 31 05:35:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082922.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 30 06:54:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.645	5969794	35.326 ug/ml
Spiked Amount 50.000		Recovery =	70.65%
12) S 1-chlorooctadecane (S...	13.066	5279162	41.019 ug/ml
Spiked Amount 50.000		Recovery =	82.04%
Target Compounds			
10) T n-Eicosane (C20)	12.625	88557	0.560 ug/ml
13) T n-Docosane (C22)	13.768	171390	1.101 ug/ml
14) T n-Tetracosane (C24)	14.924	624621	4.153 ug/ml
16) T n-Octacosane (C28)	16.869	165930	1.198 ug/ml
17) T n-Tricontane (C30)	17.752	65923	0.485 ug/ml
18) T n-Dotriacontane (C32)	18.578	62885	0.471 ug/ml
19) T n-Tetratriacontane (C34)	19.361	60456	0.478 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083022AL\
Data File : FE037338.D
Signal(s) : FID1B.ch
Acq On : 31 Aug 2022 04:52
Operator : YP\AJ
Sample : N4424-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 31 05:35:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082922.M
Quant Title : GC Extractables
QLast Update : Tue Aug 30 06:54:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

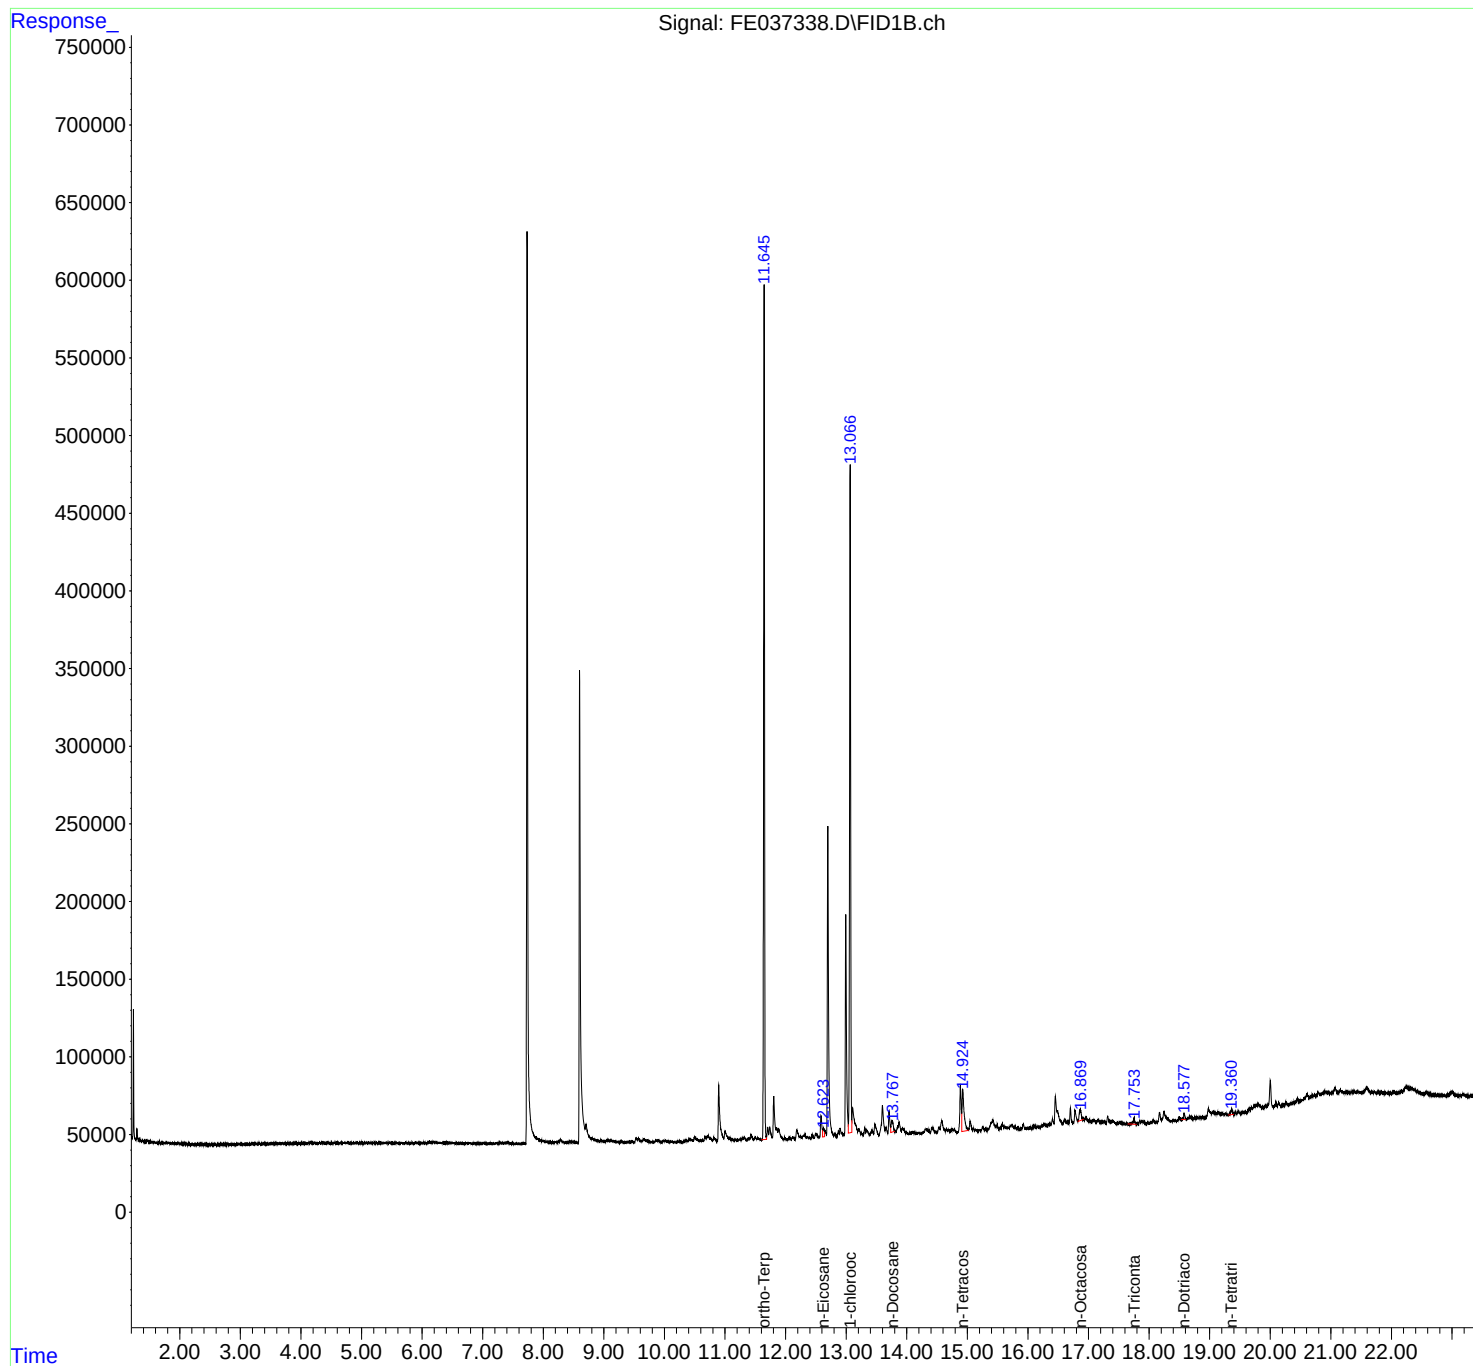


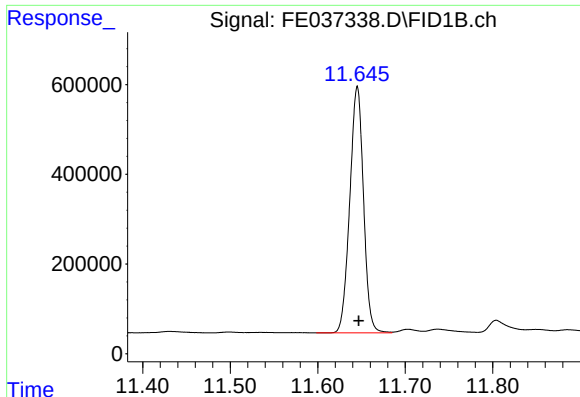

#9 ortho-Terphenyl (SURR)


R.T.: 11.645 min
Delta R.T.: -0.002 min
Response: 5969794
Conc: 35.33 ug/ml

Instrument :
FID_E
ClientSampleId :

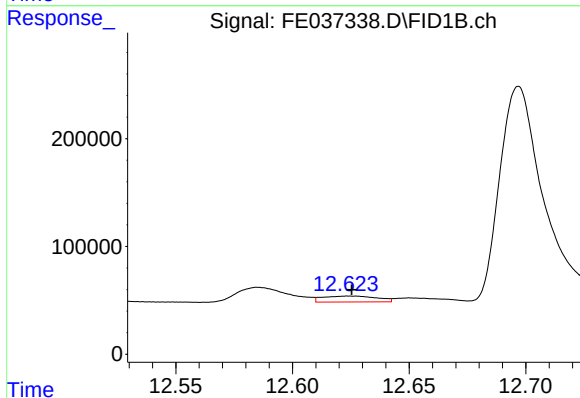


#10 n-Eicosane (C20)

R.T.: 12.625 min
Delta R.T.: 0.000 min
Response: 88557
Conc: 0.56 ug/ml

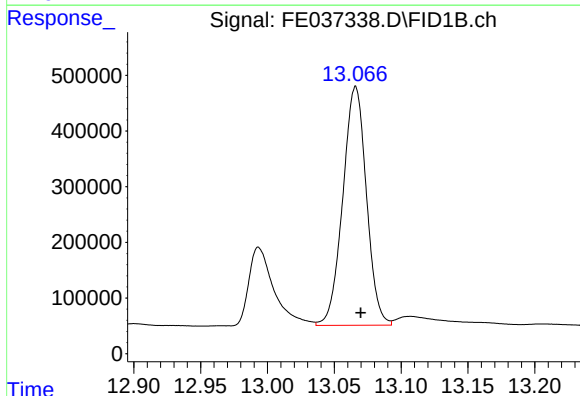


#12 1-chlorooctadecane (SURR)

R.T.: 13.066 min
Delta R.T.: -0.004 min
Response: 5279162
Conc: 41.02 ug/ml

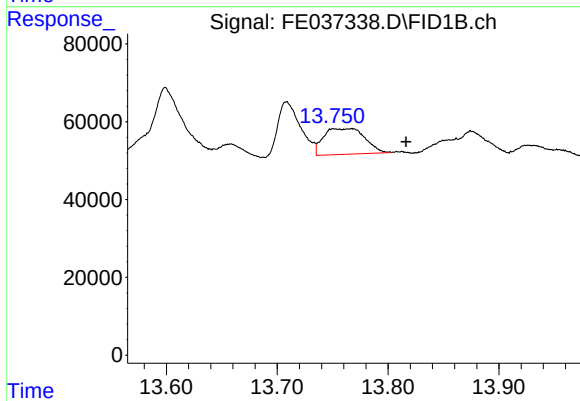

#13 n-Docosane (C22)


R.T.: 13.768 min
Delta R.T.: -0.049 min
Response: 171390
Conc: 1.10 ug/ml

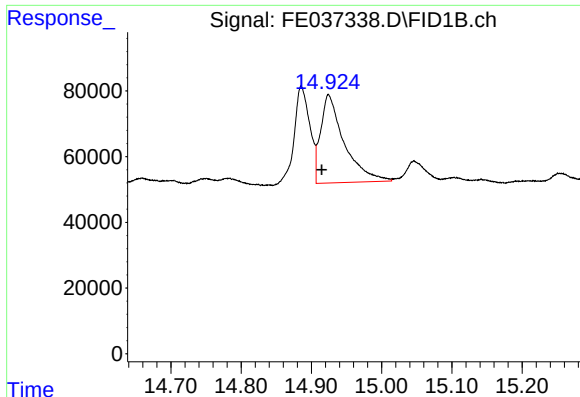

#14 n-Tetracosane (C24)


R.T.: 14.924 min
Delta R.T.: 0.010 min
Response: 624621
Conc: 4.15 ug/ml

Instrument :
FID_E
ClientSampleId :

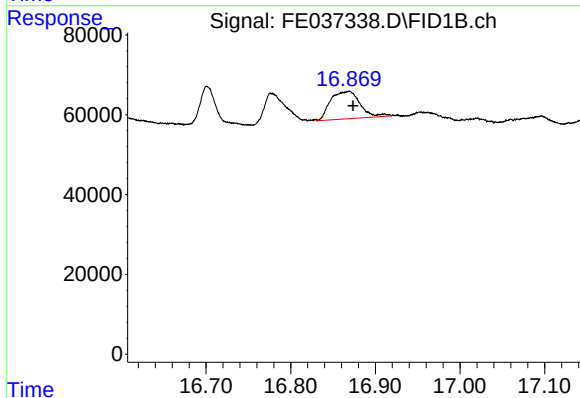


#16 n-Octacosane (C28)

R.T.: 16.869 min
Delta R.T.: -0.004 min
Response: 165930
Conc: 1.20 ug/ml

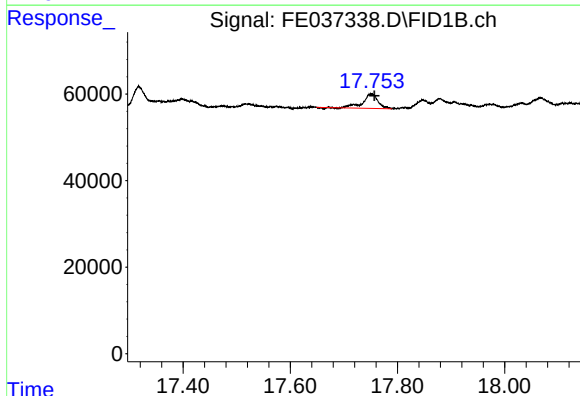


#17 n-Tricontane (C30)

R.T.: 17.752 min
Delta R.T.: -0.004 min
Response: 65923
Conc: 0.48 ug/ml

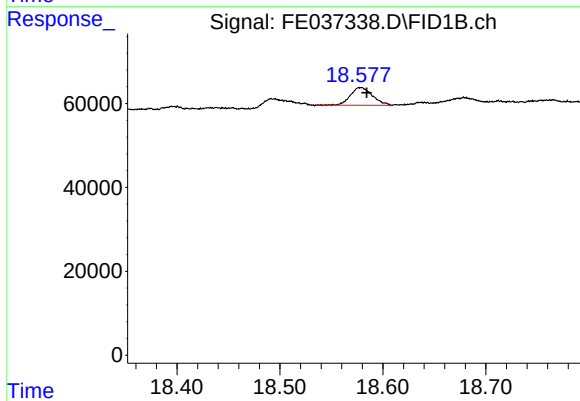

#18 n-Dotriacontane (C32)

R.T.: 18.578 min
Delta R.T.: -0.006 min
Response: 62885
Conc: 0.47 ug/ml

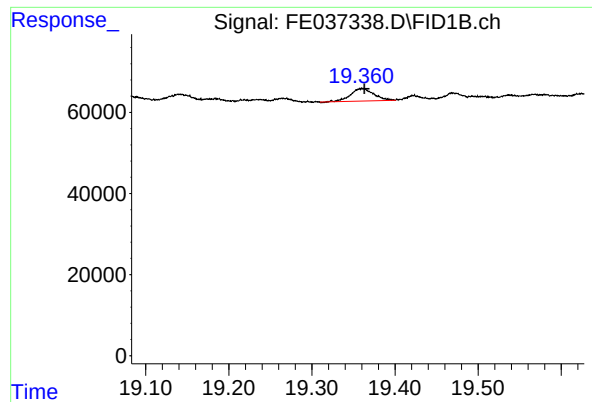

#19 n-Tetratriacontane (C34)

R.T.: 19.361 min
Delta R.T.: -0.003 min
Response: 60456
Conc: 0.48 ug/ml

Instrument :

FID_E

ClientSampleId :