

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083022AL\
 Data File : FE037347.D
 Signal(s) : FID1B.ch
 Acq On : 31 Aug 2022 09:59
 Operator : YP\AJ
 Sample : N4421-14DL2 20X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 31 10:26:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082922.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 30 06:54:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.066	186596	1.450 ug/ml
Spiked Amount 50.000		Recovery =	2.90%
Target Compounds			
10) T n-Eicosane (C20)	12.621	59927	0.379 ug/ml
16) T n-Octacosane (C28)	16.874	59642	0.431 ug/ml
18) T n-Dotriacontane (C32)	18.592	97603	0.731 ug/ml
19) T n-Tetratriacontane (C34)	19.358	112795	0.891 ug/ml
20) T n-Hexatriacontane (C36)	20.140	404279	3.143 ug/ml
21) T n-Octatriacontane (C38)	20.795	108668	0.873 ug/ml
22) T n-Tetracontane (C40)	21.604	821986	6.376 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083022AL\
Data File : FE037347.D
Signal(s) : FID1B.ch
Acq On : 31 Aug 2022 09:59
Operator : YP\AJ
Sample : N4421-14DL2 20X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 31 10:26:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 082922.M
Quant Title : GC Extractables
QLast Update : Tue Aug 30 06:54:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

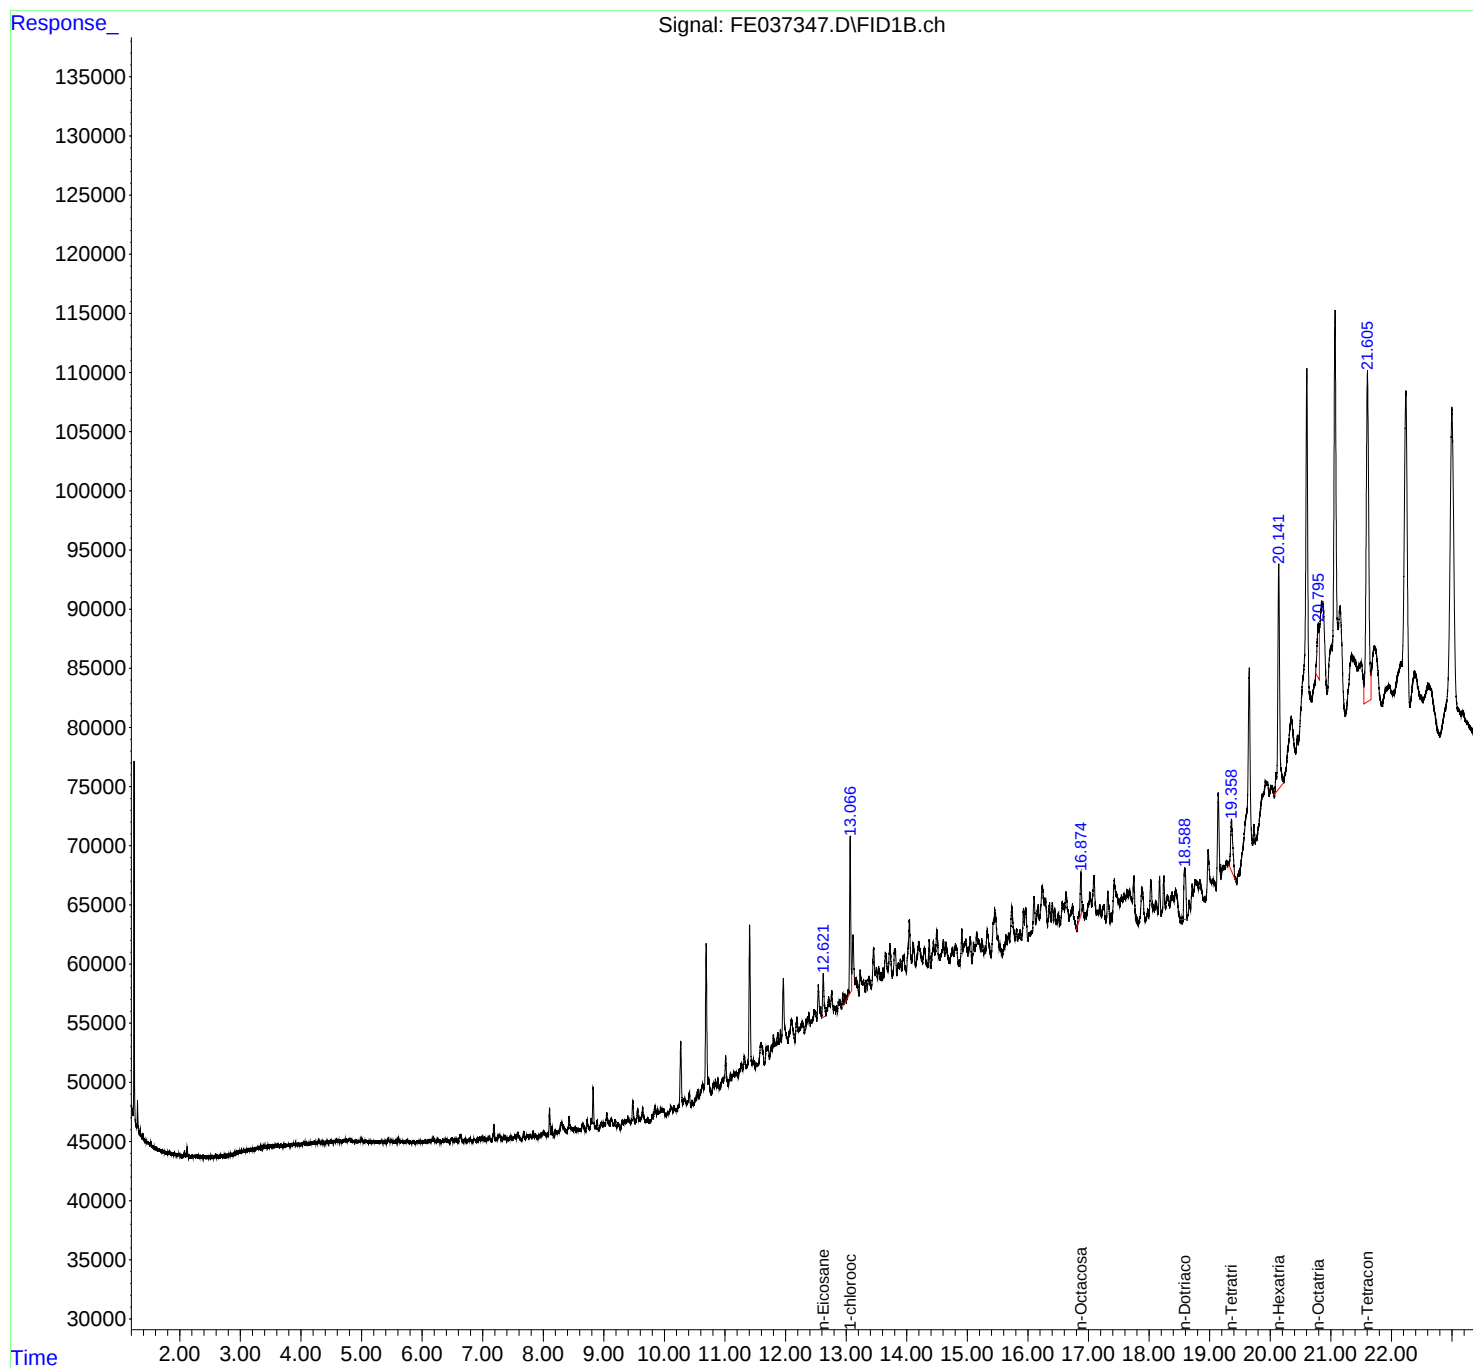


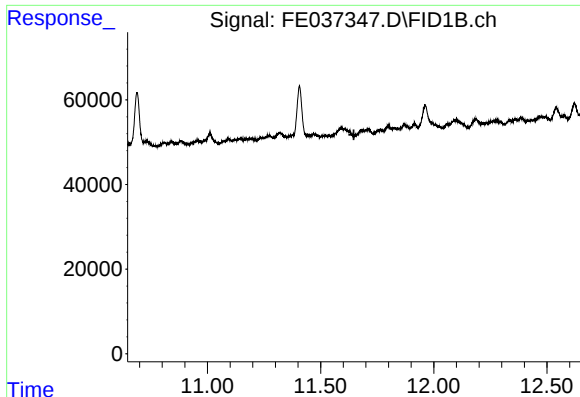

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.647 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

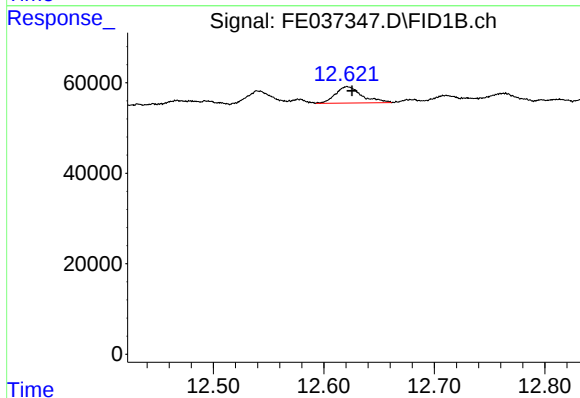


#10 n-Eicosane (C20)

R.T.: 12.621 min
Delta R.T.: -0.004 min
Response: 59927
Conc: 0.38 ug/ml

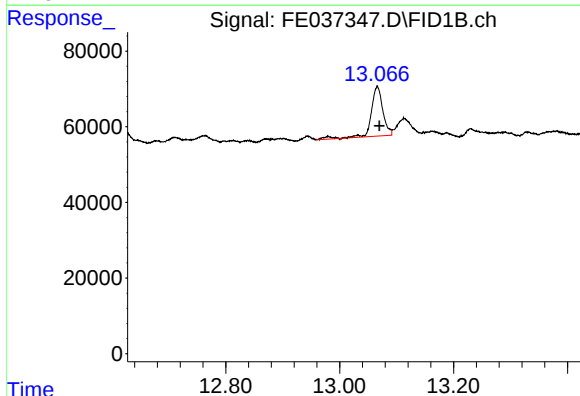


#12 1-chlorooctadecane (SURR)

R.T.: 13.066 min
Delta R.T.: -0.004 min
Response: 186596
Conc: 1.45 ug/ml

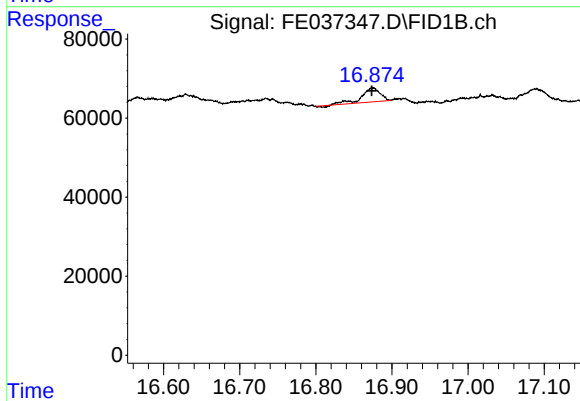

#16 n-Octacosane (C28)


R.T.: 16.874 min
Delta R.T.: 0.000 min
Response: 59642
Conc: 0.43 ug/ml

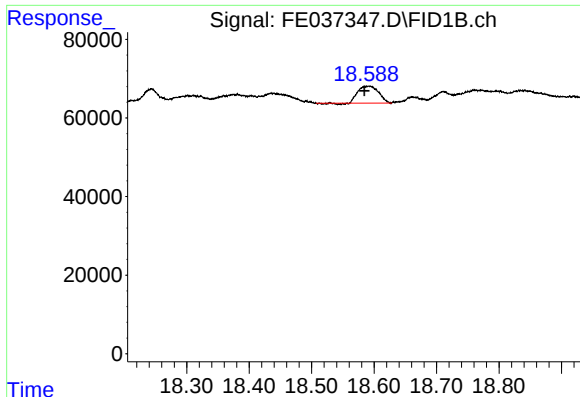

#18 n-Dotriacontane (C32)


R.T.: 18.592 min
Delta R.T.: 0.008 min
Response: 97603
Conc: 0.73 ug/ml

Instrument :
FID_E
ClientSampleId :

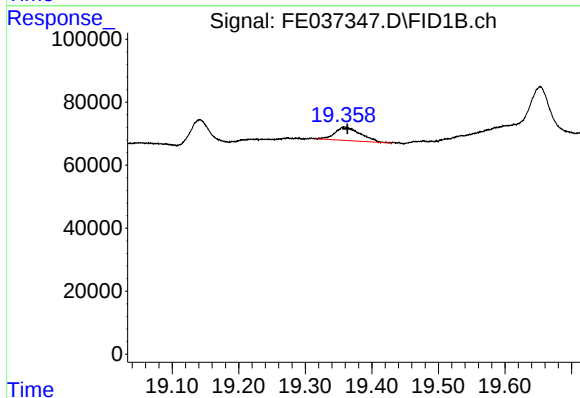


#19 n-Tetratriacontane (C34)

R.T.: 19.358 min
Delta R.T.: -0.005 min
Response: 112795
Conc: 0.89 ug/ml

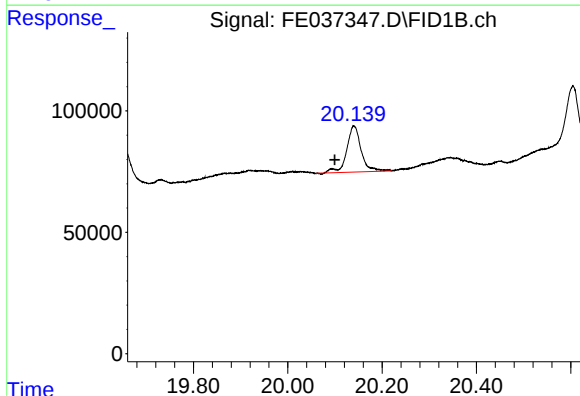


#20 n-Hexatriacontane (C36)

R.T.: 20.140 min
Delta R.T.: 0.041 min
Response: 404279
Conc: 3.14 ug/ml

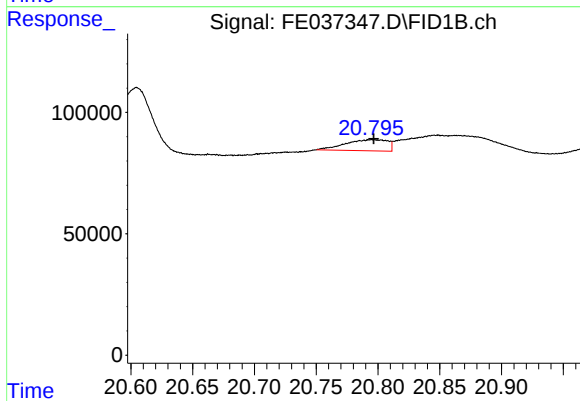

#21 n-Octatriacontane (C38)

R.T.: 20.795 min
Delta R.T.: -0.001 min
Response: 108668
Conc: 0.87 ug/ml

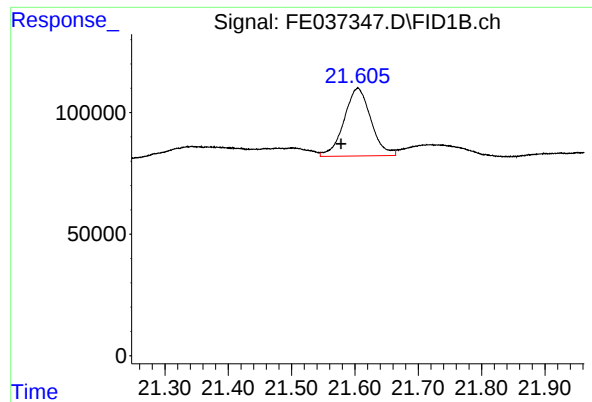

#22 n-Tetracontane (C40)

R.T.: 21.604 min
Delta R.T.: 0.026 min
Response: 821986
Conc: 6.38 ug/ml

Instrument :
FID_E
ClientSampleId :