

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE083022AL\  
Data File : FE037348.D  
Signal(s) : FID1B.ch  
Acq On : 31 Aug 2022 10:30  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Aug 31 11:06:57 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_D\methods\Aliphatic EPH 082922.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 30 06:54:11 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

| Compound                    |                         | R.T.   | Response | Conc Units   |
|-----------------------------|-------------------------|--------|----------|--------------|
| -----                       |                         |        |          |              |
| System Monitoring Compounds |                         |        |          |              |
| Target Compounds            |                         |        |          |              |
| 17) T                       | n-Tricontane (C30)      | 17.751 | 71055    | 0.522 ug/ml  |
| 18) T                       | n-Dotriacontane (C32)   | 18.596 | 283251   | 2.121 ug/ml  |
| 20) T                       | n-Hexatriacontane (C36) | 20.139 | 742067   | 5.770 ug/ml  |
| 22) T                       | n-Tetracontane (C40)    | 21.604 | 1541701  | 11.959 ug/ml |
| -----                       |                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE083022AL\  
Data File : FE037348.D  
Signal(s) : FID1B.ch  
Acq On : 31 Aug 2022 10:30  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Aug 31 11:06:57 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_D\methods\Aliphatic EPH 082922.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 30 06:54:11 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

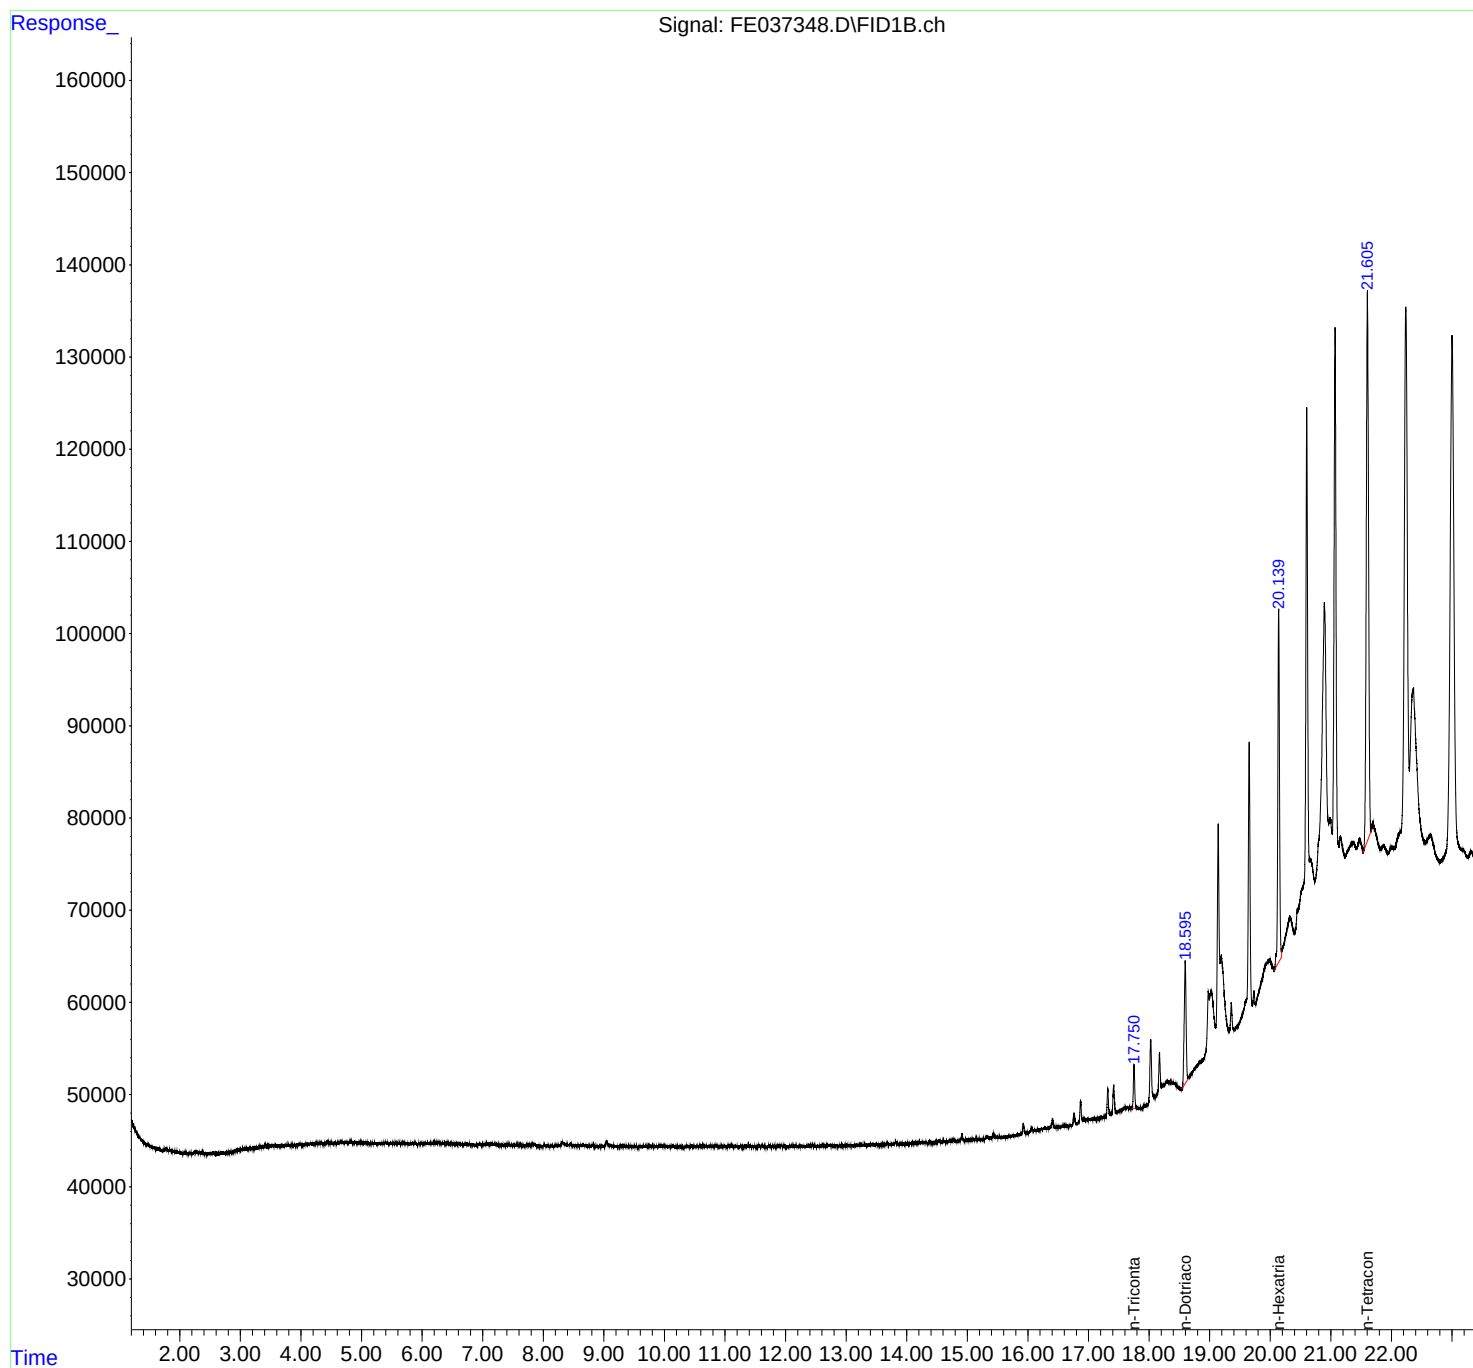


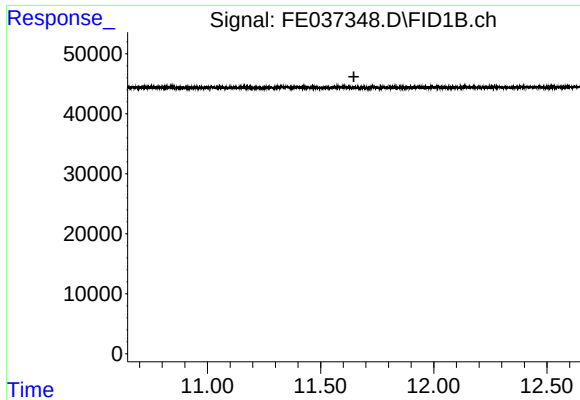

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min  
Exp R.T.: 11.647 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_E  
ClientSampleId :

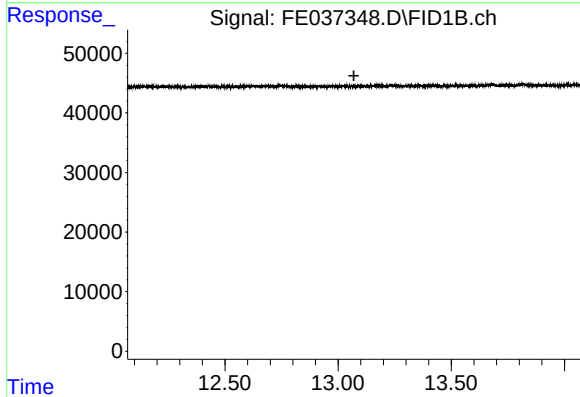


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min  
Exp R.T.: 13.070 min  
Response: 0  
Conc: N.D.

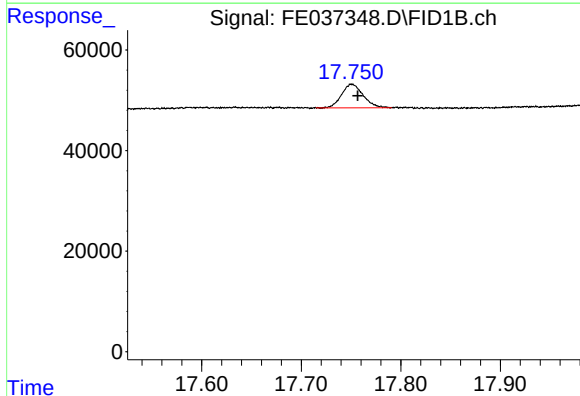


#17 n-Tricontane (C30)

R.T.: 17.751 min  
Delta R.T.: -0.006 min  
Response: 71055  
Conc: 0.52 ug/ml

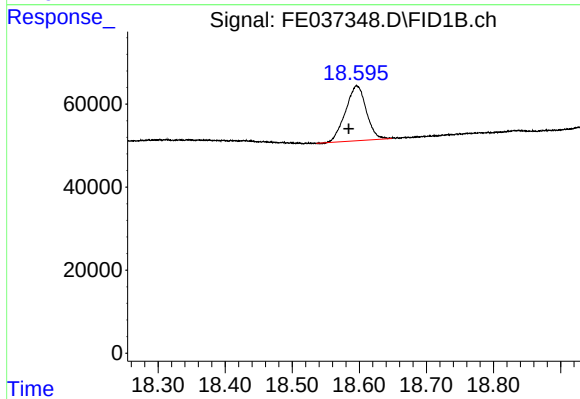

#18 n-Dotriacontane (C32)


R.T.: 18.596 min  
Delta R.T.: 0.012 min  
Response: 283251  
Conc: 2.12 ug/ml

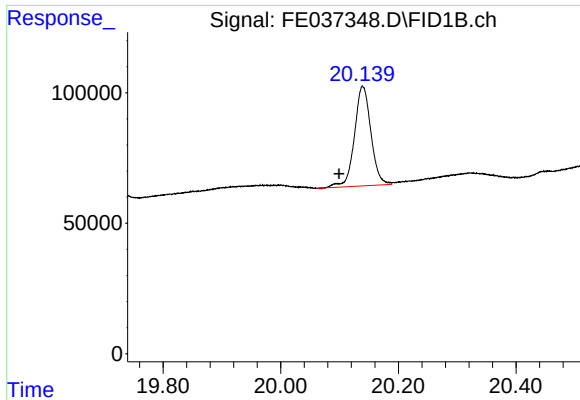

#20 n-Hexatriacontane (C36)

R.T.: 20.139 min  
Delta R.T.: 0.040 min  
Response: 742067  
Conc: 5.77 ug/ml

Instrument :  
FID\_E  
ClientSampleId :

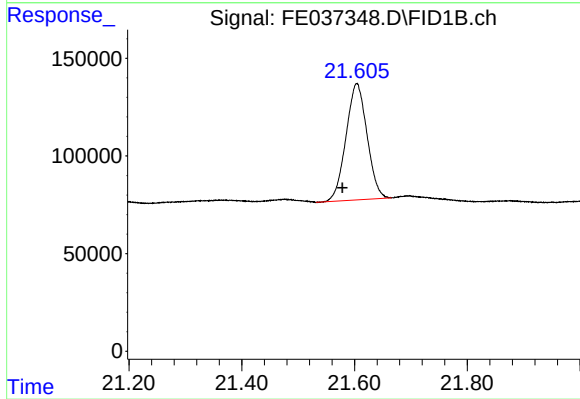

#22 n-Tetracontane (C40)

R.T.: 21.604 min  
Delta R.T.: 0.026 min  
Response: 1541701  
Conc: 11.96 ug/ml