

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE083022AL\  
 Data File : FE037346.D  
 Signal(s) : FID1B.ch  
 Acq On : 31 Aug 2022 09:28  
 Operator : YP\AJ  
 Sample : N4421-14DL 2X  
 Misc :  
 ALS Vial : 30 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 WC-PALM-SP-03-GRDL

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 08/31/2022  
 Supervised By :Ankita Jodhani 08/31/2022

Integration File: autoint1.e  
 Quant Time: Aug 31 10:08:05 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_D\methods\Aliphatic EPH 082922.M  
 Quant Title : GC Extractables  
 QLast Update : Tue Aug 30 06:54:11 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units    |
|--------------------------------|--------|------------|---------------|
| -----                          |        |            |               |
| System Monitoring Compounds    |        |            |               |
| 12) S 1-chlorooctadecane (S... | 13.067 | 1802290    | 14.004 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 28.01%        |
| Target Compounds               |        |            |               |
| -----                          |        |            |               |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE083022AL\  
Data File : FE037346.D  
Signal(s) : FID1B.ch  
Acq On : 31 Aug 2022 09:28  
Operator : YP\AJ  
Sample : N4421-14DL 2X  
Misc :  
ALS Vial : 30 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
WC-PALM-SP-03-GRDL


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 08/31/2022  
Supervised By :Ankita Jodhani 08/31/2022

Integration File: autoint1.e  
Quant Time: Aug 31 10:08:05 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_D\methods\Aliphatic EPH 082922.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 30 06:54:11 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

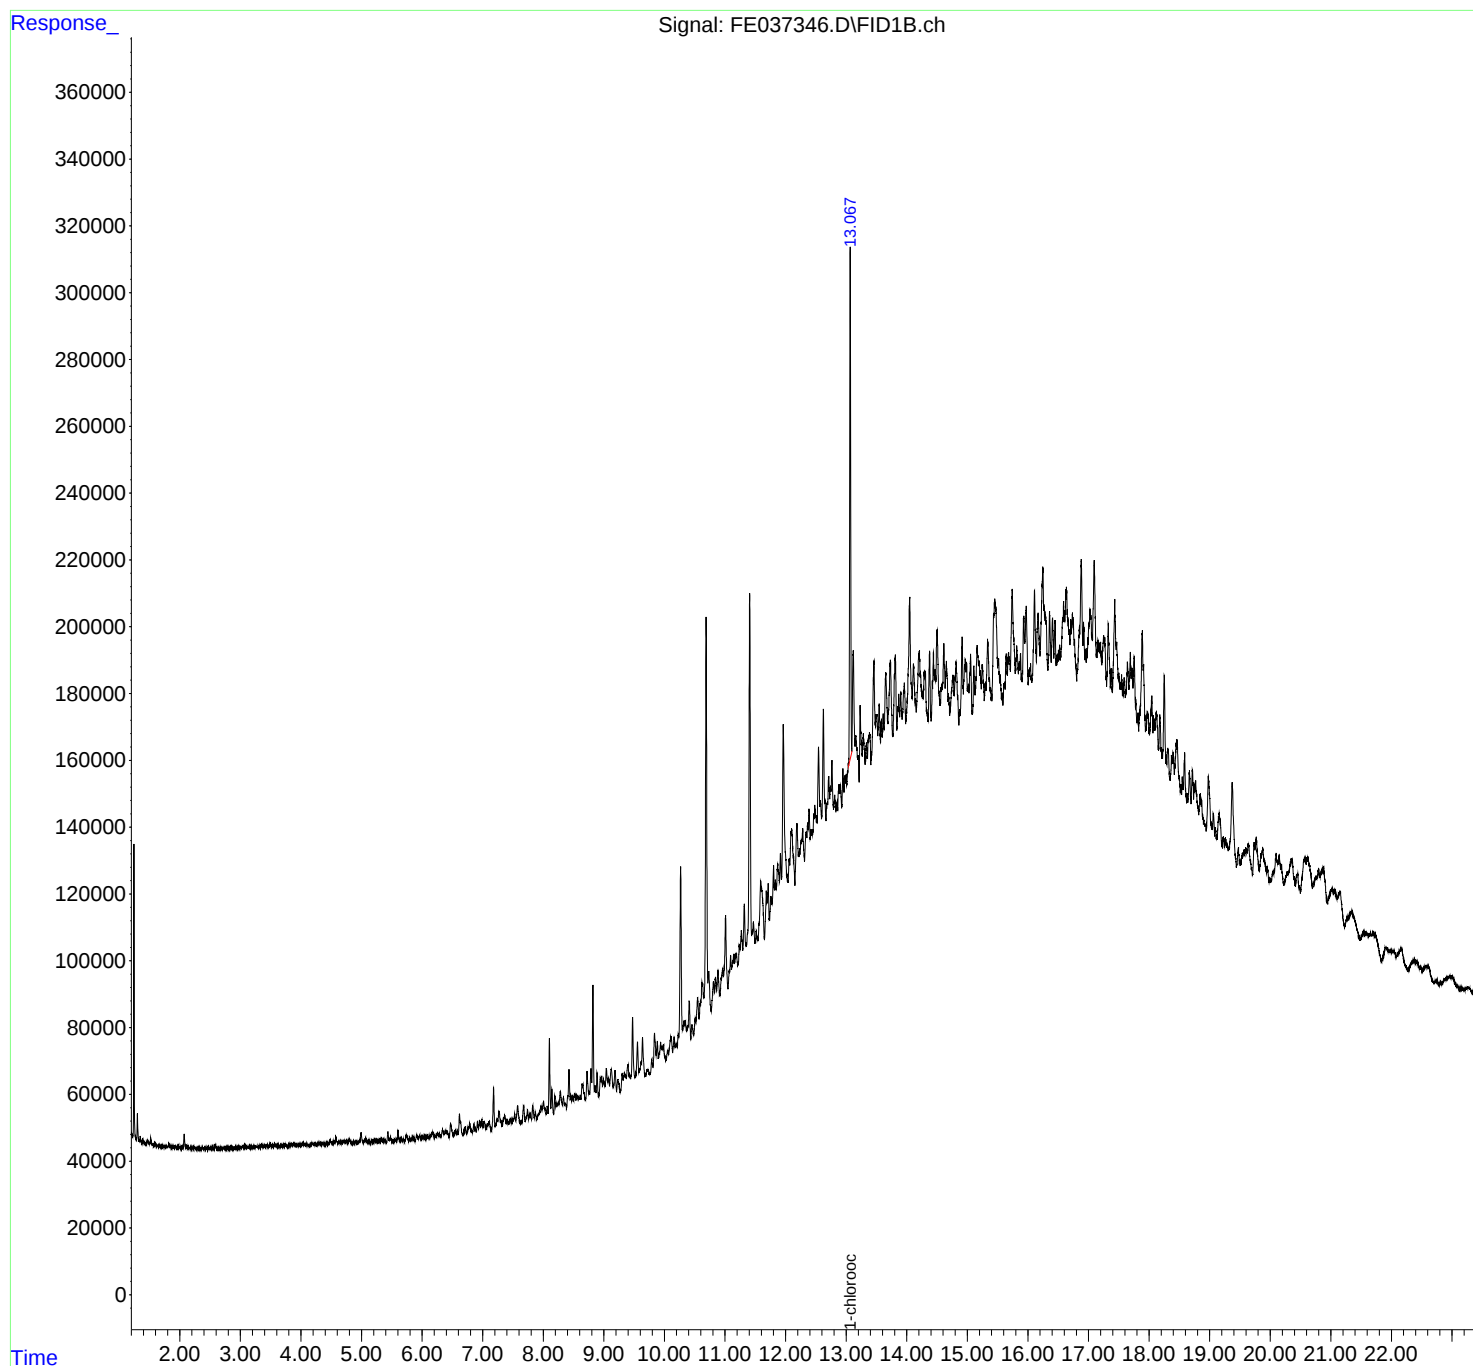

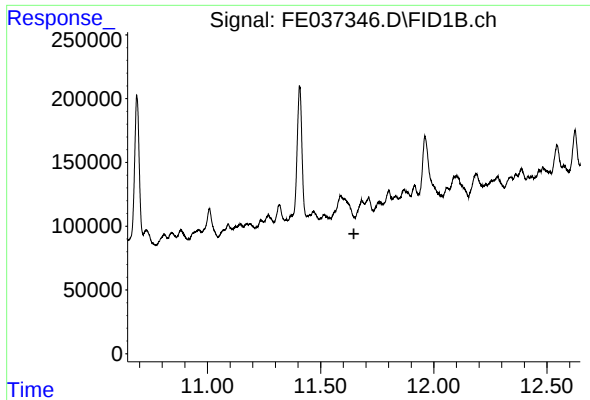


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min  
Exp R.T.: 11.647 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_E  
ClientSampleId :  
WC-PALM-SP-03-GRDL

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 08/31/2022  
Supervised By :Ankita Jodhani 08/31/2022

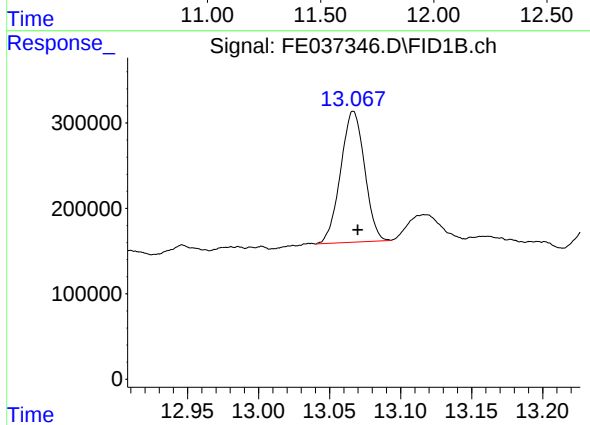

#12 1-chlorooctadecane (SURR)

R.T.: 13.067 min  
Delta R.T.: -0.003 min  
Response: 1802290  
Conc: 14.00 ug/ml m