

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083120\
 Data File : FE032654.D
 Signal(s) : FID1B.CH
 Acq On : 31 Aug 2020 13:29
 Operator : DD\AJ
 Sample : L3832-10 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 RW-M-20200827

Integration File: autoint1.e
 Quant Time: Sep 01 00:36:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE081120.M
 Quant Title :
 QLast Update : Thu Aug 13 11:46:52 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.688	724047	2.250 ug/ml
Target Compounds			
4) N-TETRADECANE	8.308	55678	0.154 ug/ml
5) N-HEXADECANE	9.871	678616	1.860 ug/ml
6) N-OCTADECANE	11.250f	566872	1.526 ug/ml
16) N-HEXATRIACONTANE	20.102	51770	0.230 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083120\
Data File : FE032654.D
Signal(s) : FID1B.CH
Acq On : 31 Aug 2020 13:29
Operator : DD\AJ
Sample : L3832-10 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
RW-M-20200827

Integration File: autoint1.e
Quant Time: Sep 01 00:36:52 2020
Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE081120.M
Quant Title :
QLast Update : Thu Aug 13 11:46:52 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

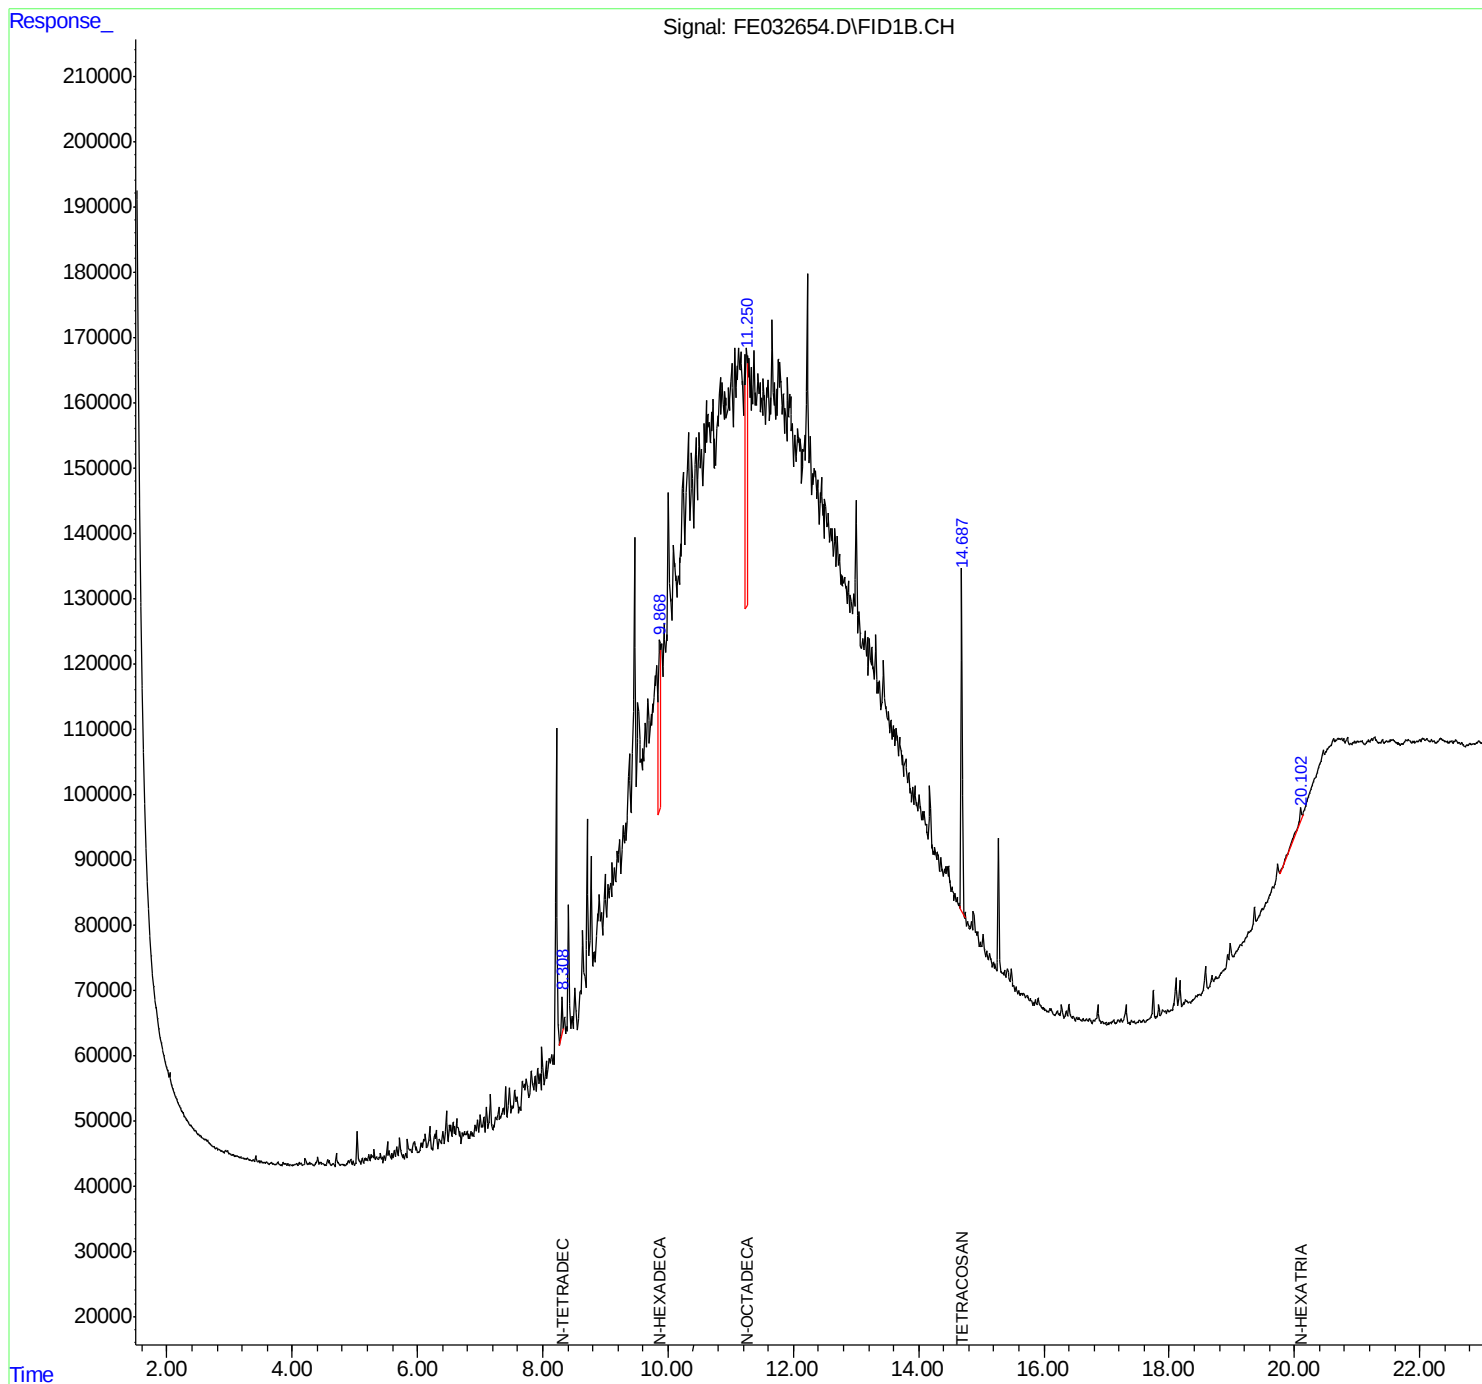


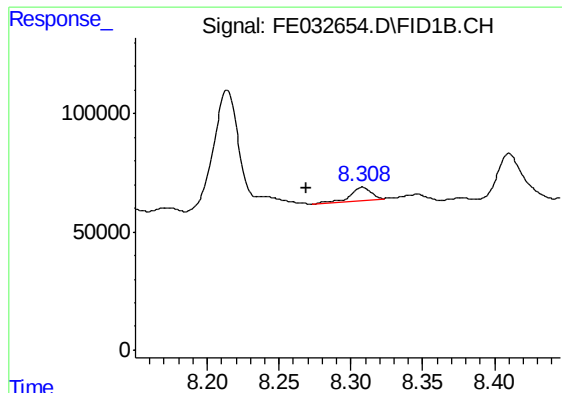

#4 N-TETRADECANE


R.T.: 8.308 min
Delta R.T.: 0.039 min
Response: 55678
Conc: 0.15 ug/ml

Instrument :
FID_E
ClientSampleId :
RW-M-20200827

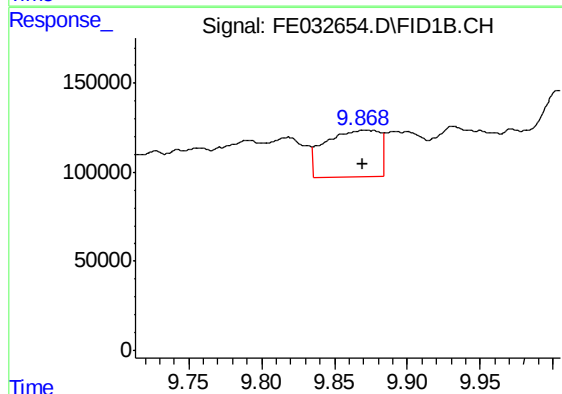


#5 N-HEXADECANE

R.T.: 9.871 min
Delta R.T.: 0.002 min
Response: 678616
Conc: 1.86 ug/ml

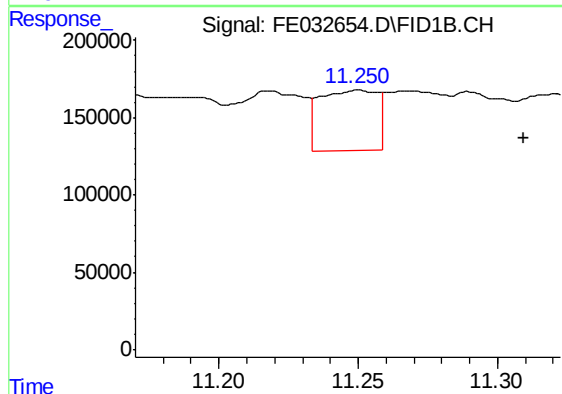


#6 N-OCTADECANE

R.T.: 11.250 min
Delta R.T.: -0.059 min
Response: 566872
Conc: 1.53 ug/ml

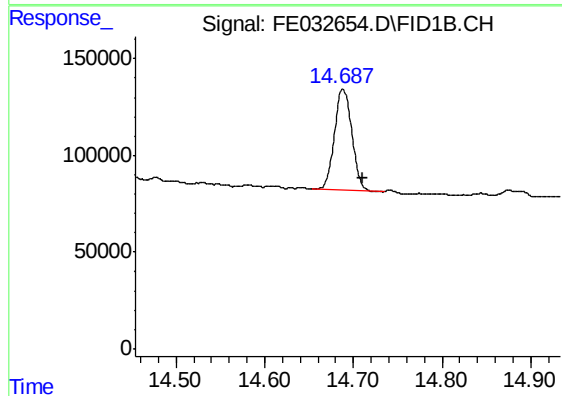

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.688 min
Delta R.T.: -0.023 min
Response: 724047
Conc: 2.25 ug/ml

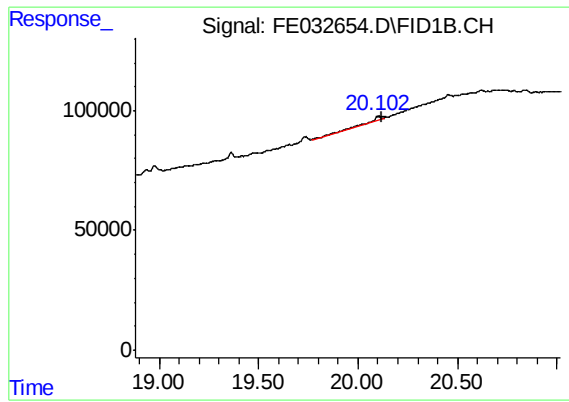

#16 N-HEXATRIACONTANE

R.T.: 20.102 min
Delta R.T.: -0.016 min
Response: 51770
Conc: 0.23 ug/ml

Instrument :
FID_E
ClientSampleId :
RW-M-20200827