

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083122\
Data File : FE037353.D
Signal(s) : FID1B.ch
Acq On : 31 Aug 2022 13:09
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 01 09:26:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE082922.M
Quant Title :
QLast Update : Mon Aug 29 16:06:19 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.467	3012684	18.515 ug/ml
12)	N-OCTACOSANE	16.869	2848355	18.487 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083122\
Data File : FE037353.D
Signal(s) : FID1B.ch
Acq On : 31 Aug 2022 13:09
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 01 09:26:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE082922.M
Quant Title :
QLast Update : Mon Aug 29 16:06:19 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

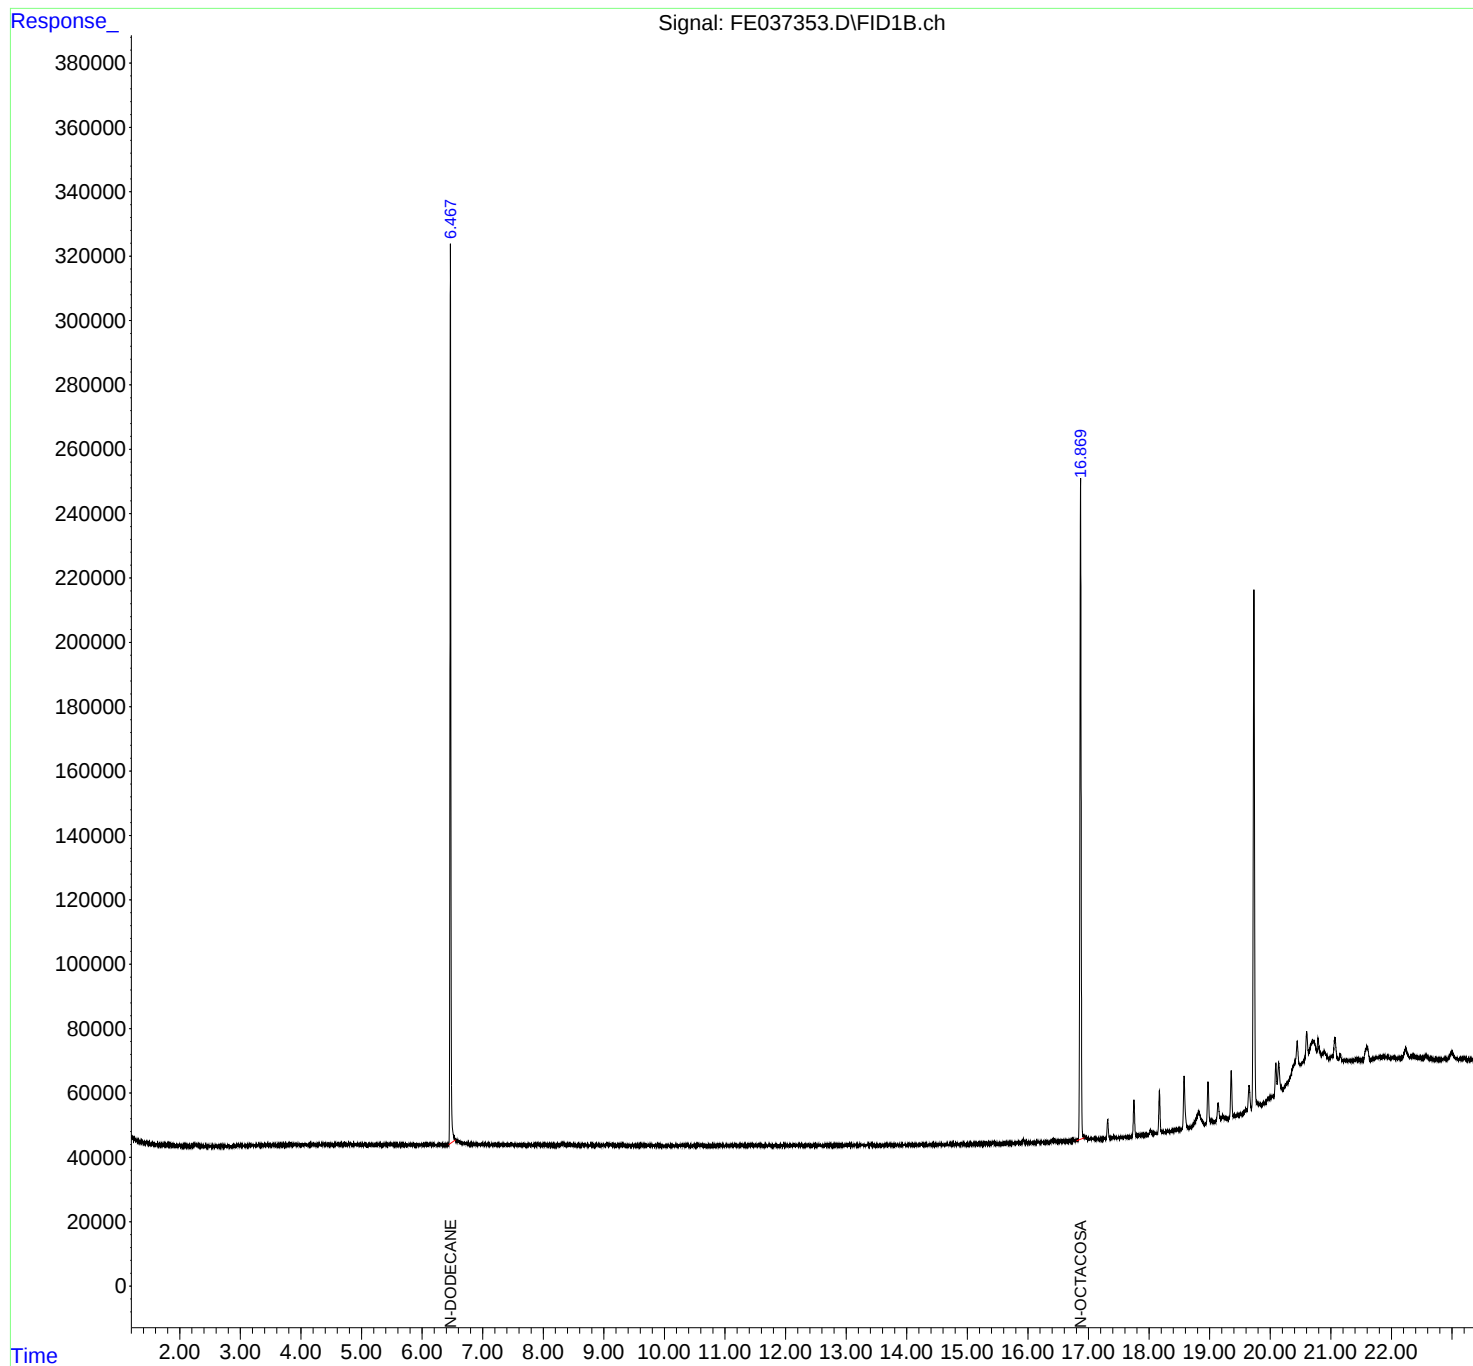


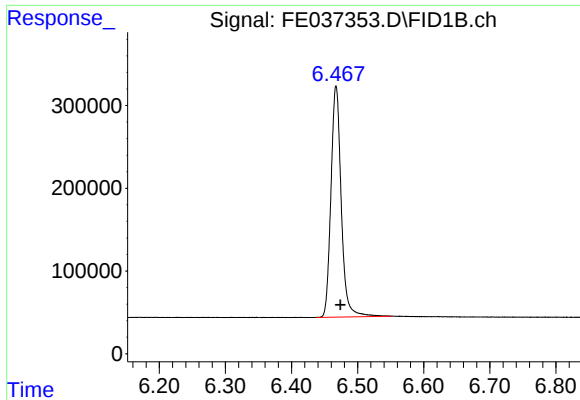

#3 N-DODECANE


R.T.: 6.467 min
Delta R.T.: -0.007 min
Response: 3012684
Conc: 18.52 ug/ml

Instrument :
FID_E
ClientSampleId :
RT MARKER

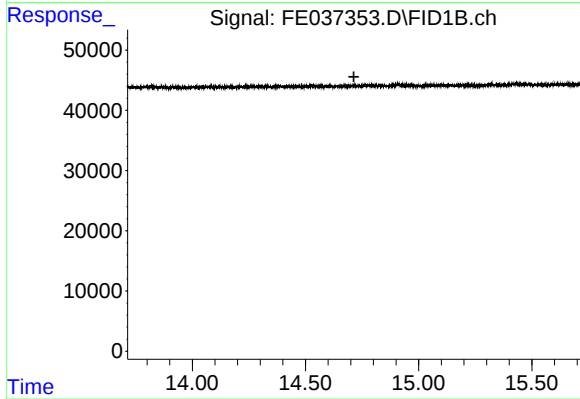

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.714 min
Response: 0
Conc: N.D.

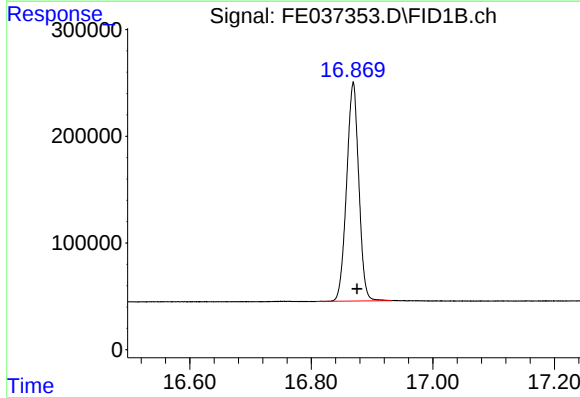

#12 N-OCTACOSANE

R.T.: 16.869 min
Delta R.T.: -0.006 min
Response: 2848355
Conc: 18.49 ug/ml