

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083122\
Data File : FE037363.D
Signal(s) : FID1B.ch
Acq On : 31 Aug 2022 18:50
Operator : YP\AJ
Sample : PB146675BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB146675BL

Integration File: autoint1.e
Quant Time: Sep 01 09:27:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE082922.M
Quant Title :
QLast Update : Mon Aug 29 16:06:19 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.707	3252450	22.702 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083122\
Data File : FE037363.D
Signal(s) : FID1B.ch
Acq On : 31 Aug 2022 18:50
Operator : YP\AJ
Sample : PB146675BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB146675BL

Integration File: autoint1.e
Quant Time: Sep 01 09:27:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE082922.M
Quant Title :
QLast Update : Mon Aug 29 16:06:19 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

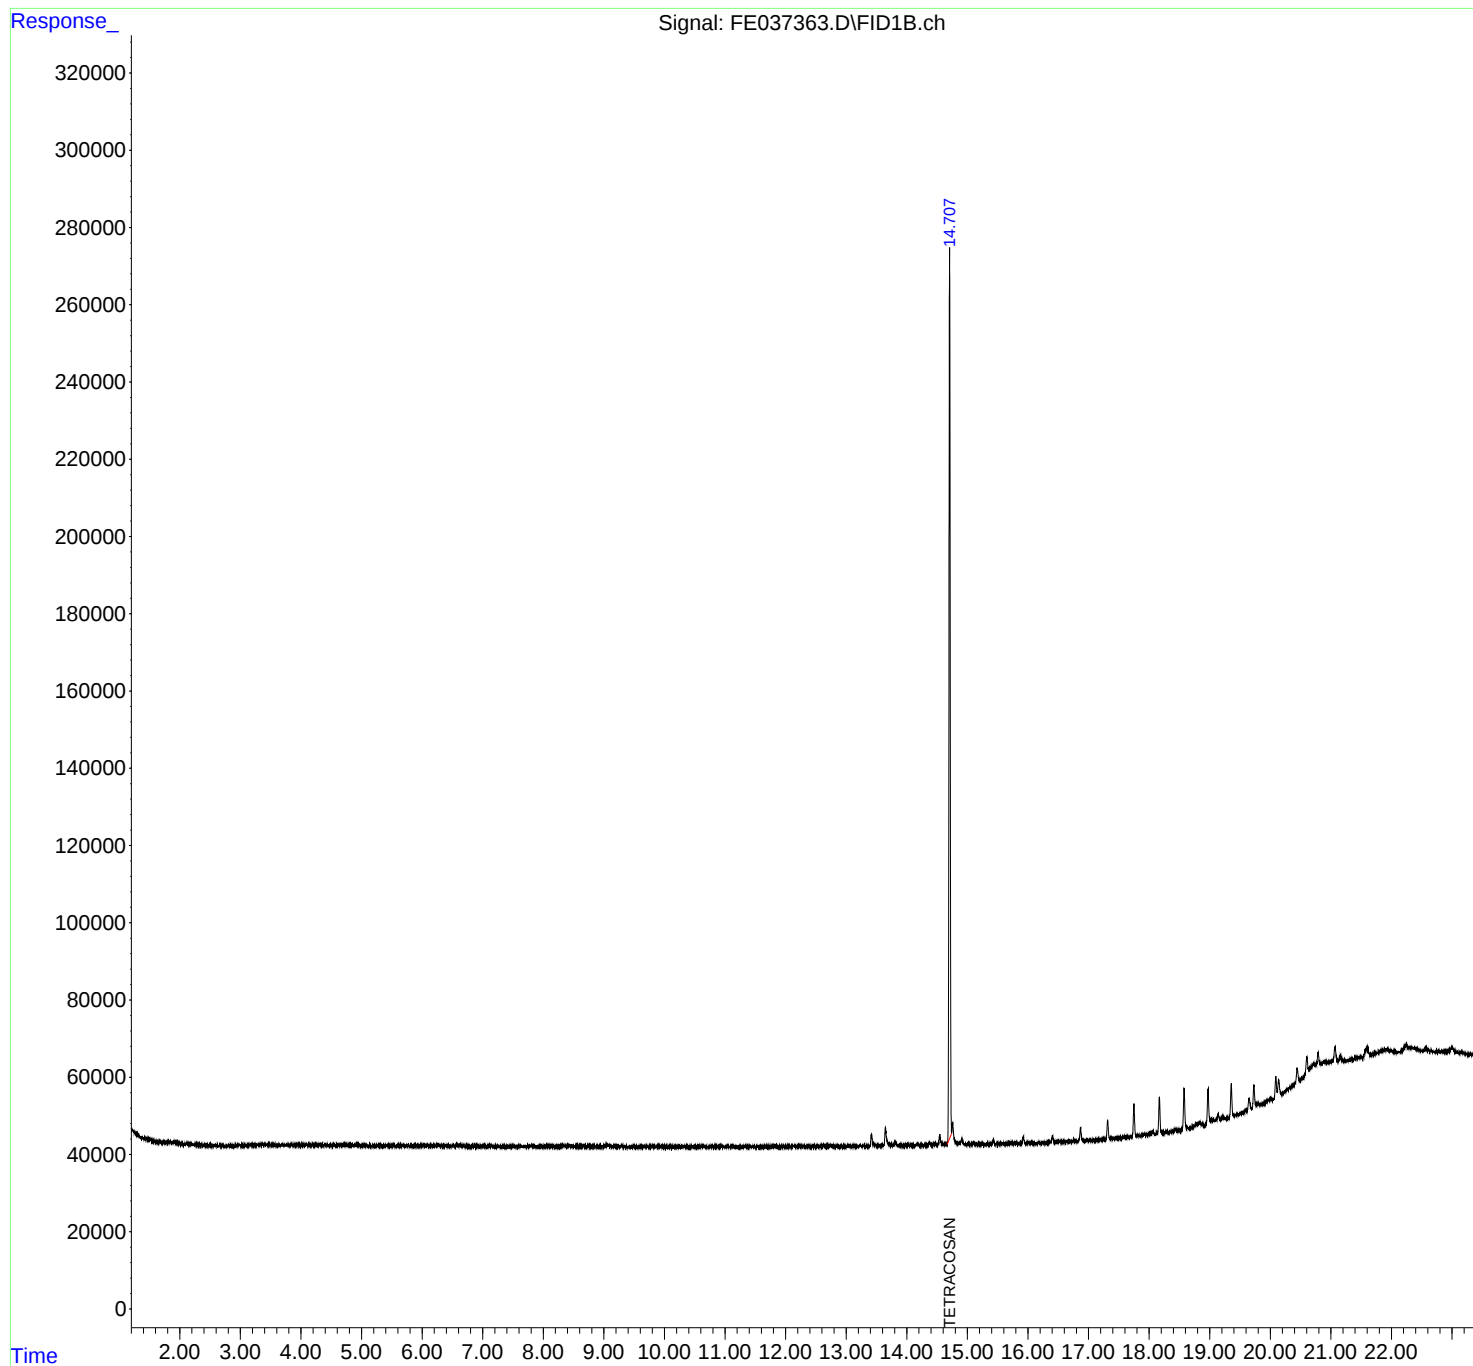

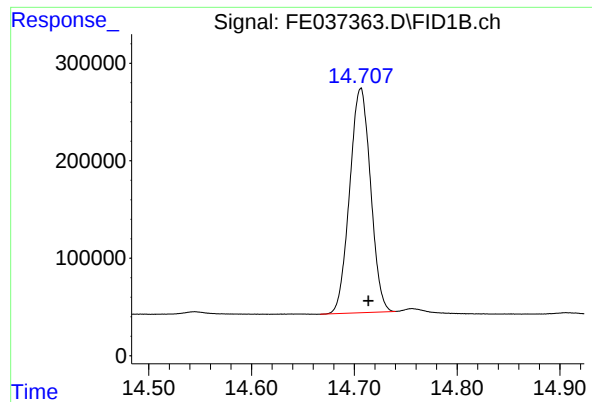

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.707 min
Delta R.T.: -0.007 min
Response: 3252450
Conc: 22.70 ug/ml

Instrument :
FID_E
ClientSampleId :
PB146675BL