

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083122\
Data File : FE037364.D
Signal(s) : FID1B.ch
Acq On : 31 Aug 2022 19:21
Operator : YP\AJ
Sample : PB146680BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB146680BL

Integration File: autoint1.e
Quant Time: Sep 01 09:27:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE082922.M
Quant Title :
QLast Update : Mon Aug 29 16:06:19 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.705	2999020	20.933 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083122\
Data File : FE037364.D
Signal(s) : FID1B.ch
Acq On : 31 Aug 2022 19:21
Operator : YP\AJ
Sample : PB146680BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB146680BL

Integration File: autoint1.e
Quant Time: Sep 01 09:27:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE082922.M
Quant Title :
QLast Update : Mon Aug 29 16:06:19 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

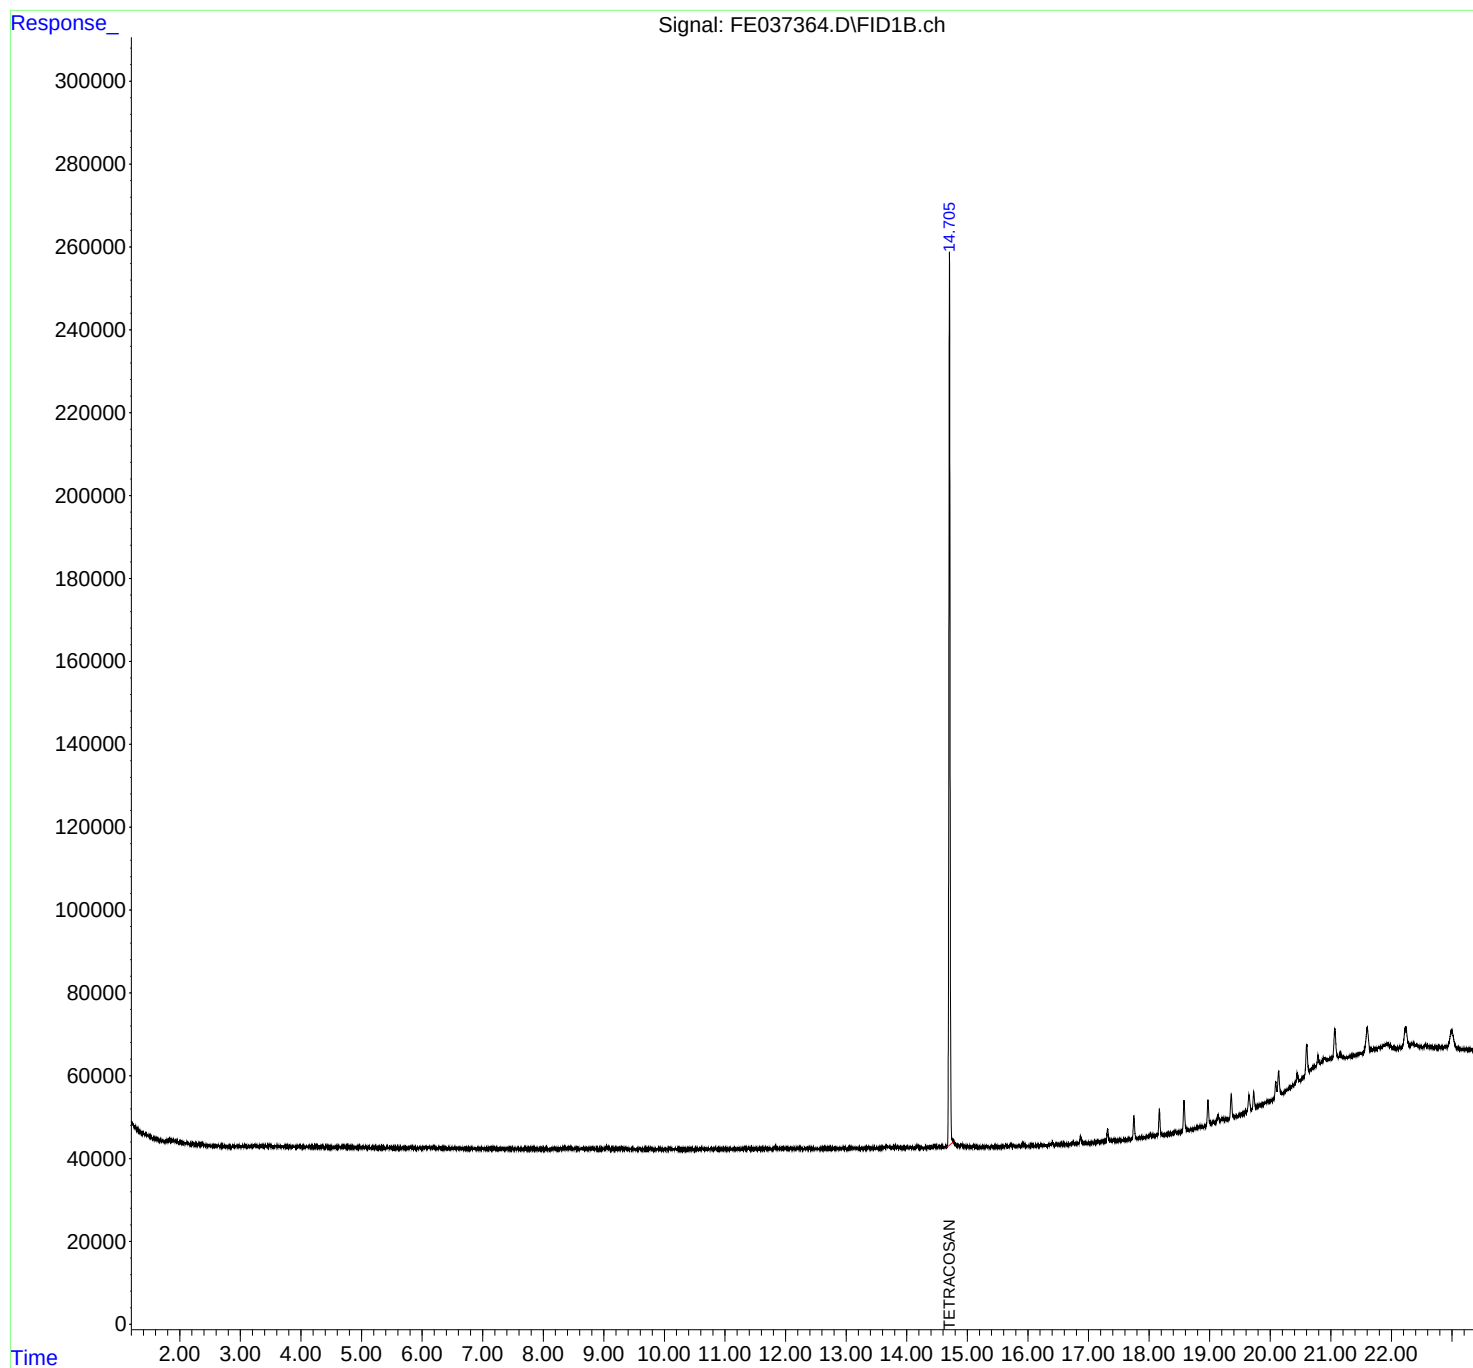

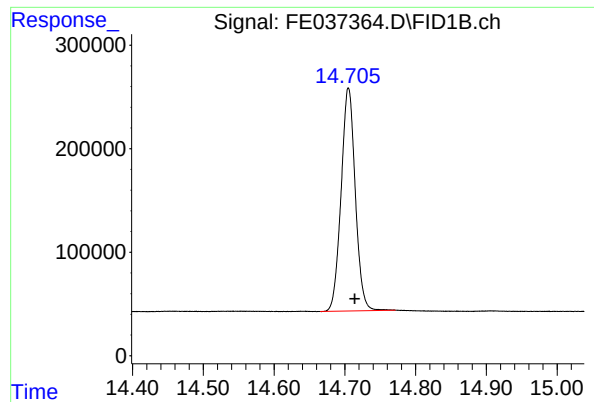

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.705 min
Delta R.T.: -0.009 min
Response: 2999020
Conc: 20.93 ug/ml

Instrument :
FID_E
ClientSampleId :
PB146680BL