

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083123\
Data File : FE044051.D
Signal(s) : FID1B.ch
Acq On : 31 Aug 2023 08:44
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 01 00:24:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE083023.M
Quant Title :
QLast Update : Thu Aug 31 02:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.027	2520447	17.192 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.925	49677	0.365 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083123\
Data File : FE044051.D
Signal(s) : FID1B.ch
Acq On : 31 Aug 2023 08:44
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 01 00:24:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE083023.M
Quant Title :
QLast Update : Thu Aug 31 02:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

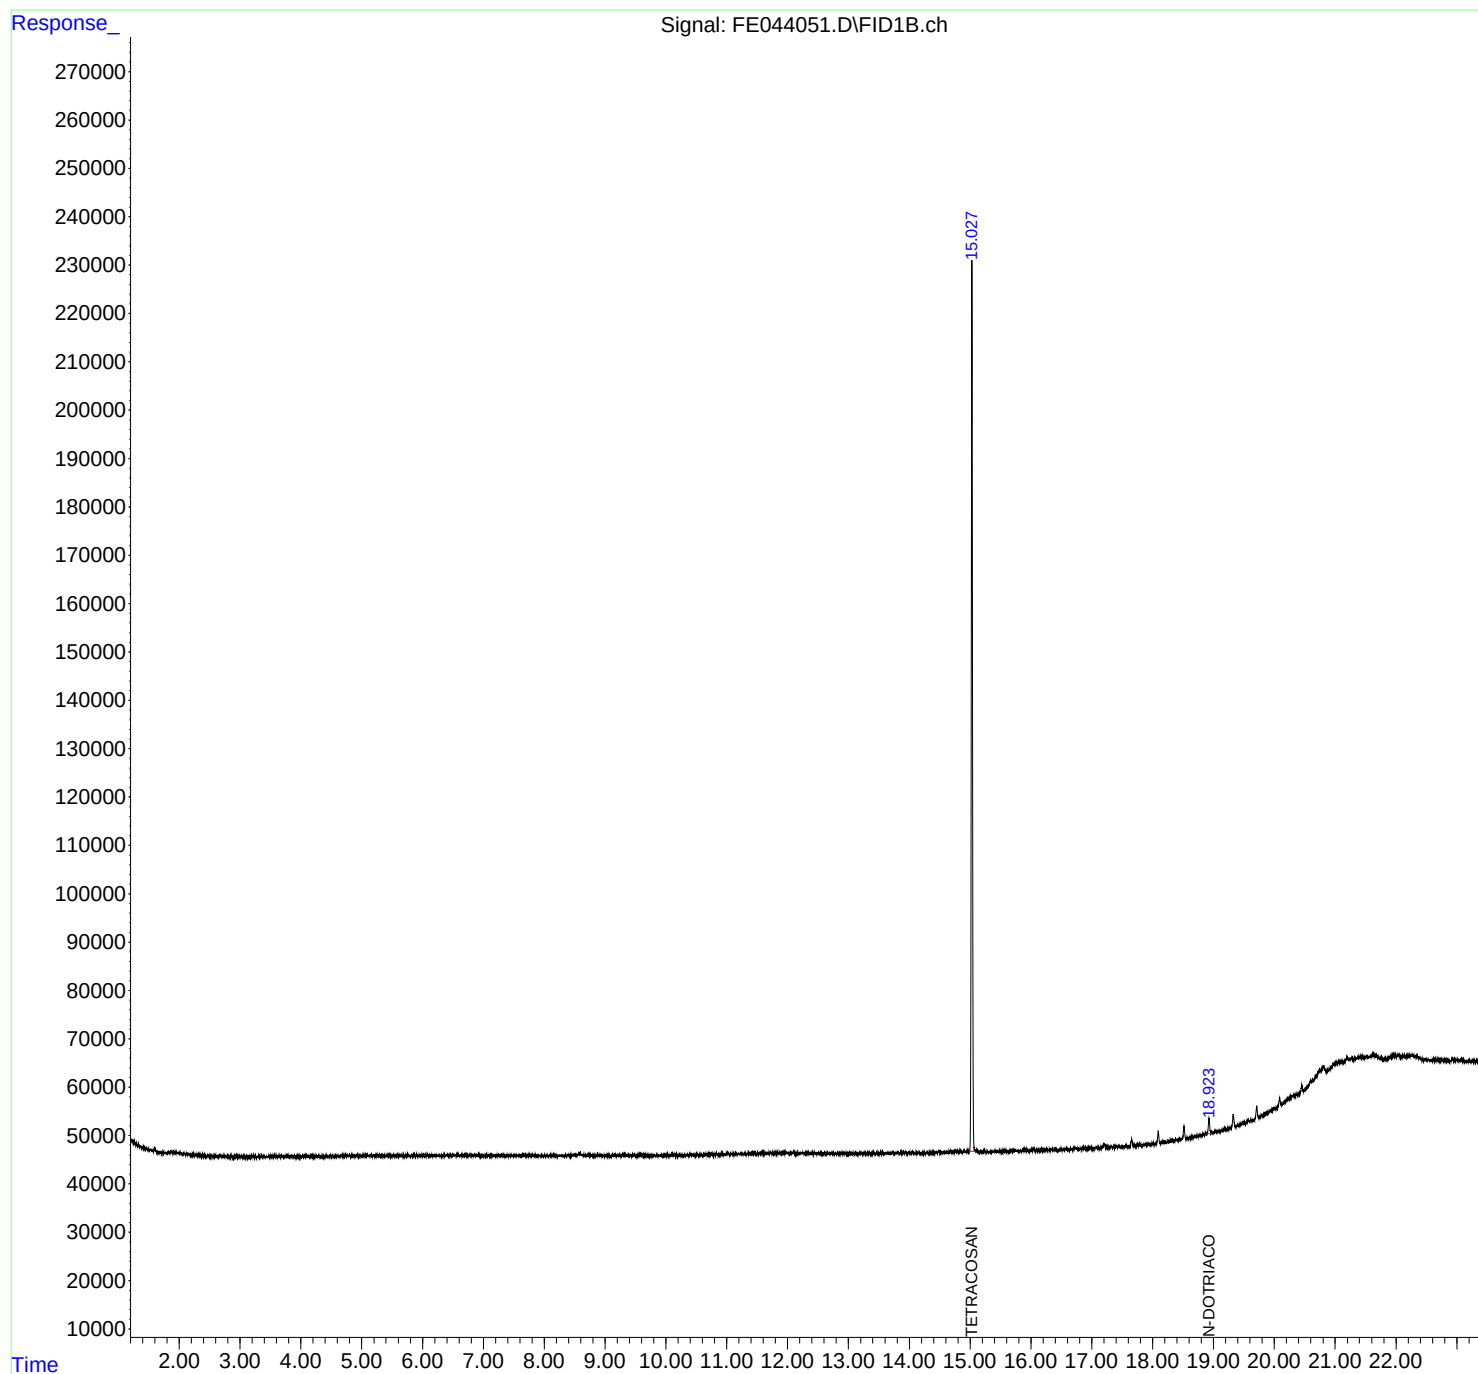


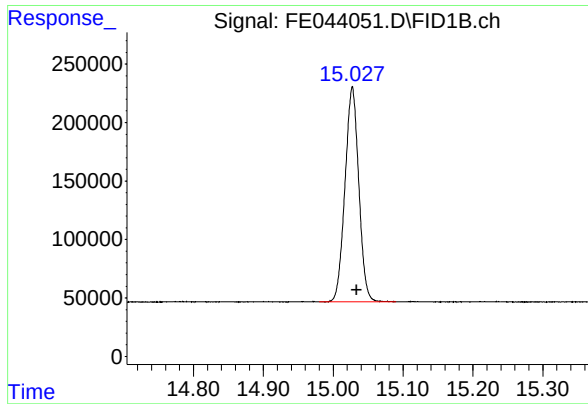

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.027 min
Delta R.T.: -0.006 min
Response: 2520447
Conc: 17.19 ug/ml

Instrument :
FID_E
ClientSampleId :

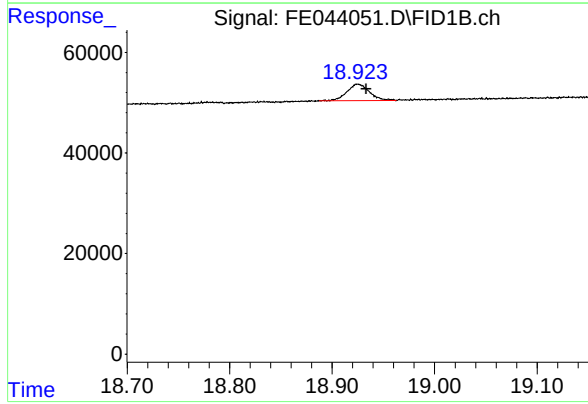

#14 N-DOTRIACONTANE

R.T.: 18.925 min
Delta R.T.: -0.009 min
Response: 49677
Conc: 0.37 ug/ml