

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083123\
 Data File : FE044065.D
 Signal(s) : FID1B.ch
 Acq On : 31 Aug 2023 16:55
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Sep 01 00:26:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE083023.M
 Quant Title :
 QLast Update : Thu Aug 31 02:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.029	6971937	47.555 ug/ml
Target Compounds			
2) N-DECANE	4.573	8130783	48.225 ug/ml
3) N-DODECANE	6.739	8239393	48.368 ug/ml
4) N-TETRADECANE	8.566	8305005	48.280 ug/ml
5) N-HEXADECANE	10.174	8364783	48.510 ug/ml
6) N-OCTADECANE	11.618	8406567	48.389 ug/ml
7) N-EICOSANE	12.930	8192069	47.978 ug/ml
8) N-DOCOSANE	14.128	7952002	47.334 ug/ml
10) N-TETRACOSANE	15.232	7840488	47.484 ug/ml
11) N-HEXACOSANE	16.255	7633017	47.462 ug/ml
12) N-OCTACOSANE	17.204	7420197	47.464 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083123\
Data File : FE044065.D
Signal(s) : FID1B.ch
Acq On : 31 Aug 2023 16:55
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Sep 01 00:26:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE083023.M
Quant Title :
QLast Update : Thu Aug 31 02:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

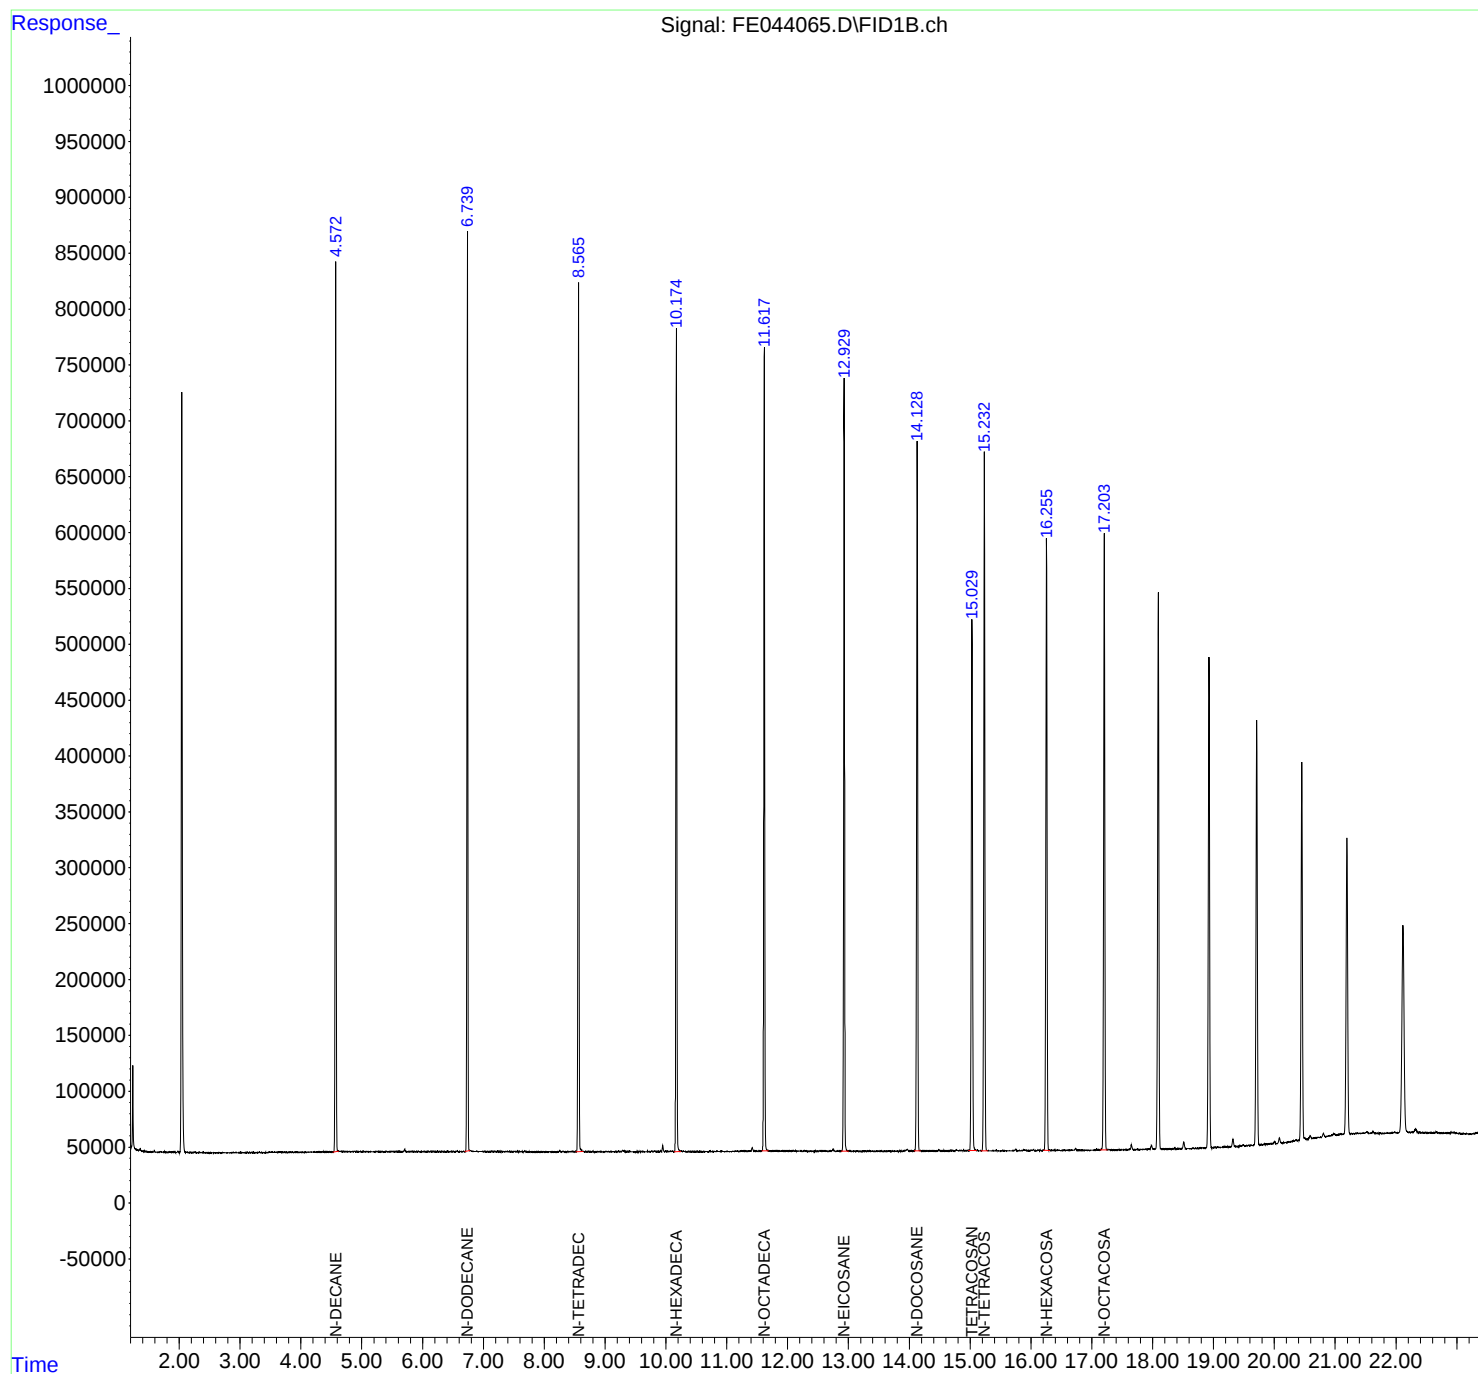


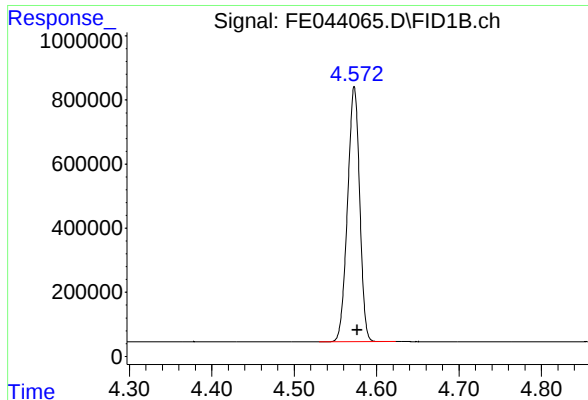

#2 N-DECANE


R.T.: 4.573 min
Delta R.T.: -0.003 min
Response: 8130783
Conc: 48.22 ug/ml

Instrument :
FID_E
ClientSampleId :
50 PPM TRPH STD

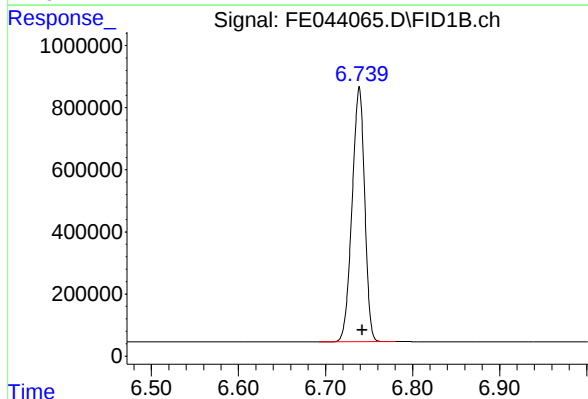


#3 N-DODECANE

R.T.: 6.739 min
Delta R.T.: -0.003 min
Response: 8239393
Conc: 48.37 ug/ml

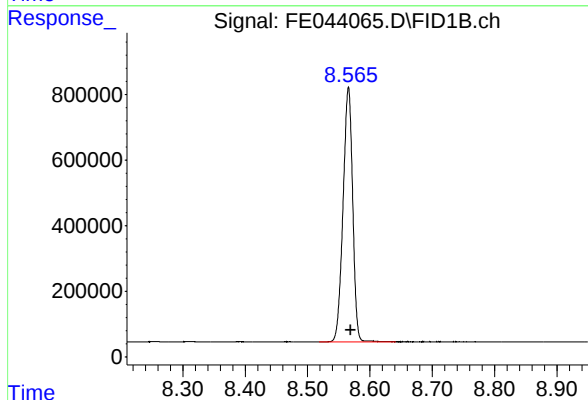


#4 N-TETRADECANE

R.T.: 8.566 min
Delta R.T.: -0.004 min
Response: 8305005
Conc: 48.28 ug/ml

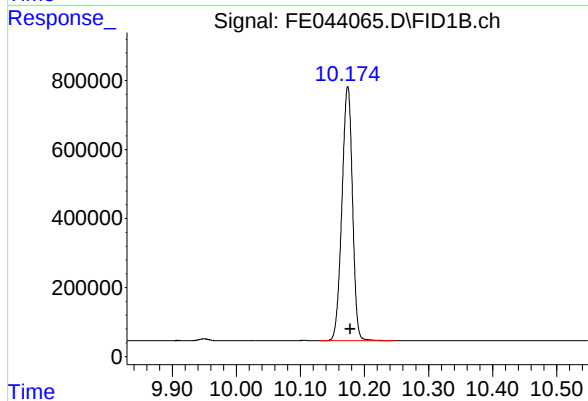

#5 N-HEXADECANE


R.T.: 10.174 min
Delta R.T.: -0.004 min
Response: 8364783
Conc: 48.51 ug/ml

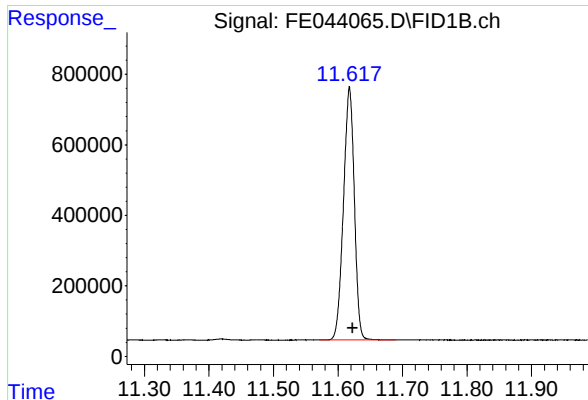

#6 N-OCTADECANE


R.T.: 11.618 min
Delta R.T.: -0.005 min
Response: 8406567
Conc: 48.39 ug/ml

Instrument :
FID_E
ClientSampleId :
50 PPM TRPH STD

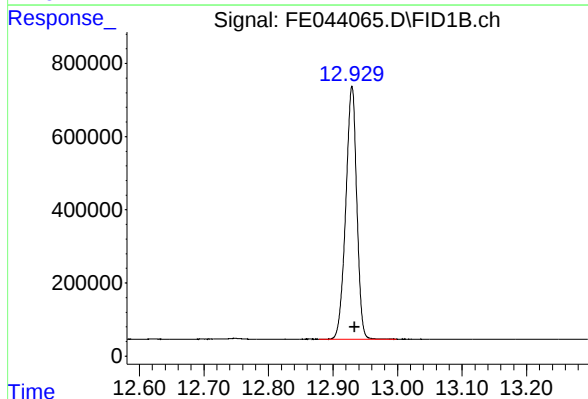


#7 N-EICOSANE

R.T.: 12.930 min
Delta R.T.: -0.004 min
Response: 8192069
Conc: 47.98 ug/ml

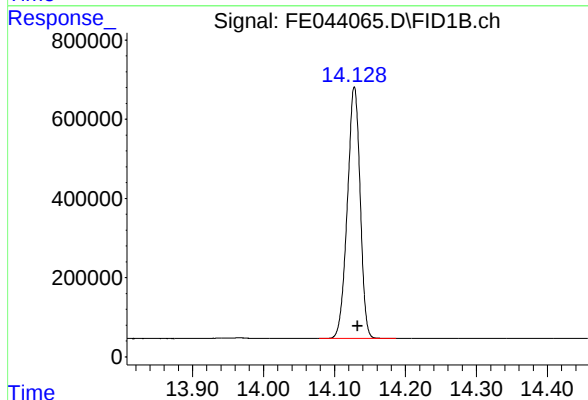


#8 N-DOCOSANE

R.T.: 14.128 min
Delta R.T.: -0.005 min
Response: 7952002
Conc: 47.33 ug/ml

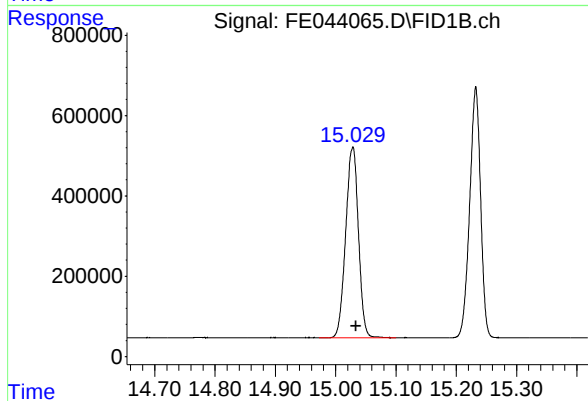

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.029 min
Delta R.T.: -0.005 min
Response: 6971937
Conc: 47.56 ug/ml

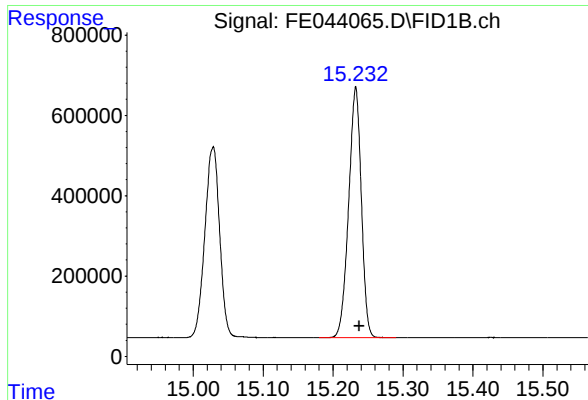

#10 N-TETRACOSANE


R.T.: 15.232 min
Delta R.T.: -0.005 min
Response: 7840488
Conc: 47.48 ug/ml

Instrument :
FID_E
ClientSampleId :
50 PPM TRPH STD

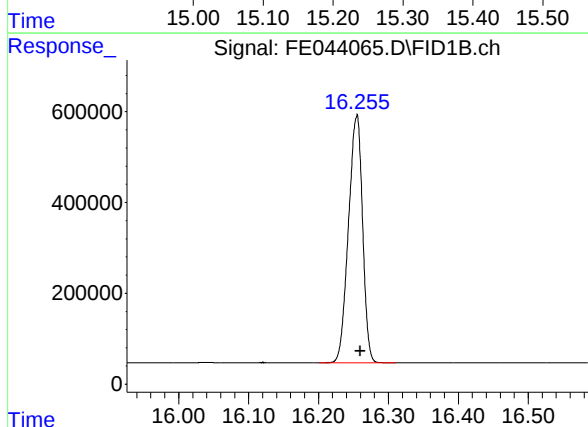

#11 N-HEXACOSANE

R.T.: 16.255 min
Delta R.T.: -0.005 min
Response: 7633017
Conc: 47.46 ug/ml

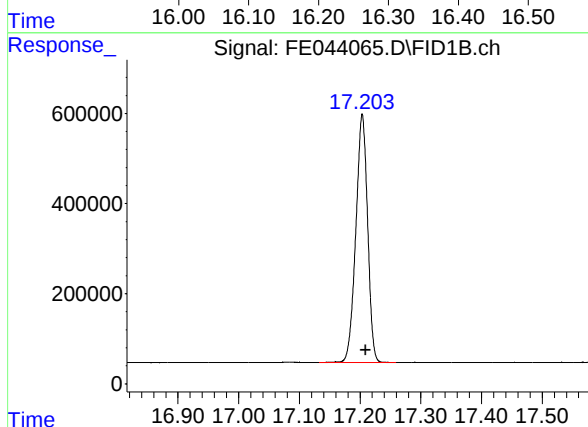

#12 N-OCTACOSANE

R.T.: 17.204 min
Delta R.T.: -0.006 min
Response: 7420197
Conc: 47.46 ug/ml