

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083123\
Data File : FE044068.D
Signal(s) : FID1B.ch
Acq On : 31 Aug 2023 18:58
Operator : YP\AJ
Sample : PB154659BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB154659BL

Integration File: autoint1.e
Quant Time: Sep 01 00:26:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE083023.M
Quant Title :
QLast Update : Thu Aug 31 02:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.026	2662900	18.163 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083123\
Data File : FE044068.D
Signal(s) : FID1B.ch
Acq On : 31 Aug 2023 18:58
Operator : YP\AJ
Sample : PB154659BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB154659BL

Integration File: autoint1.e
Quant Time: Sep 01 00:26:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE083023.M
Quant Title :
QLast Update : Thu Aug 31 02:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

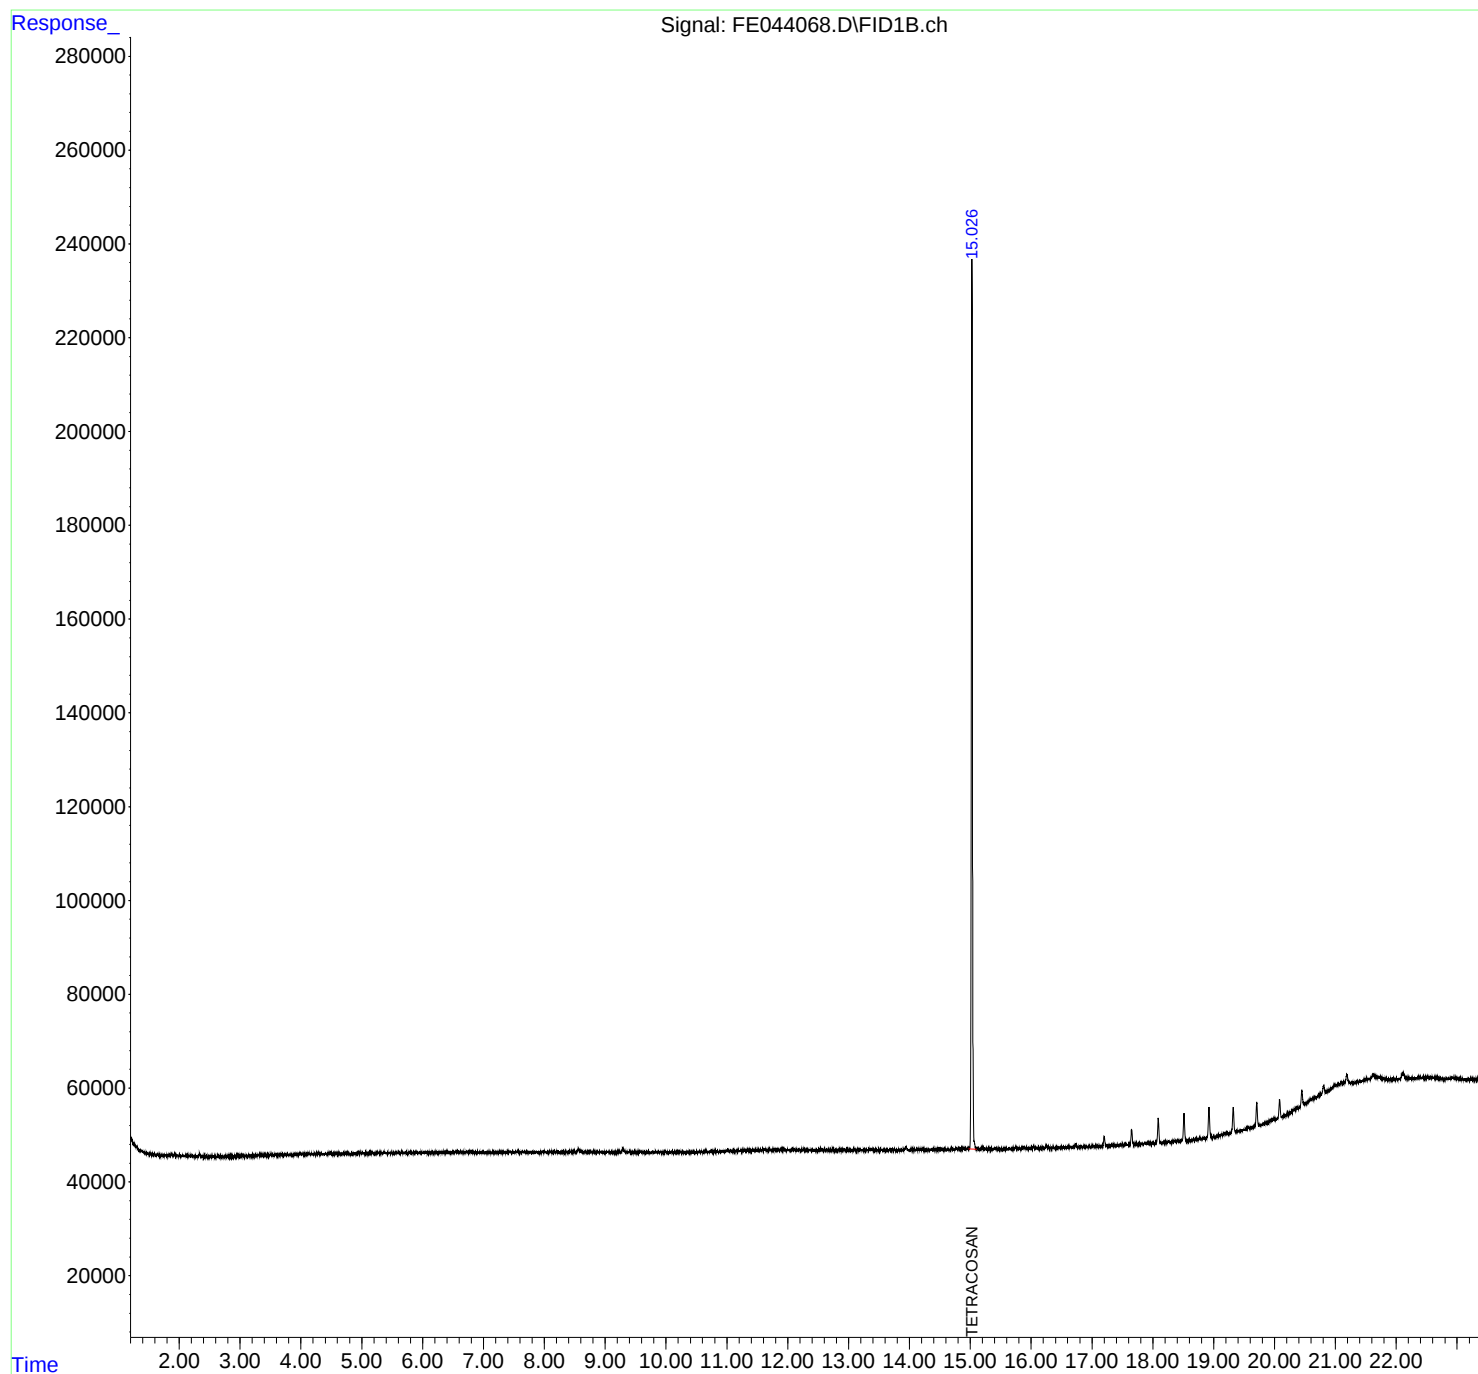

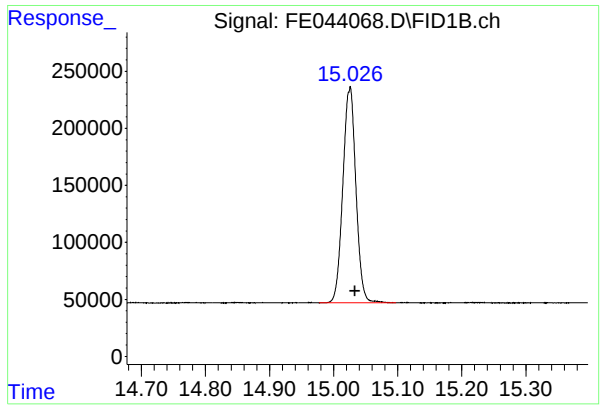

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.026 min
Delta R.T.: -0.008 min
Response: 2662900
Conc: 18.16 ug/ml

Instrument :
FID_E
ClientSampleId :
PB154659BL