

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083124AL\
 Data File : FE049836.D
 Signal(s) : FID1B.ch
 Acq On : 30 Aug 2024 06:08
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 MECL2

Integration File: autoint1.e
 Quant Time: Aug 31 04:12:30 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 081424.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 14 11:05:17 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

10) T	n-Eicosane (C20)	12.857	104858	0.702 ug/ml
11) T	n-Heneicosane (C21)	13.477	245910	1.676 ug/ml
13) T	n-Docosane (C22)	14.060	27193	0.187 ug/ml
14) T	n-Tetracosane (C24)	15.163	86165	0.592 ug/ml
15) T	n-Hexacosane (C26)	16.198	179149	1.241 ug/ml
16) T	n-Octacosane (C28)	17.132	102277	0.710 ug/ml
17) T	n-Tricontane (C30)	18.019	99194	0.663 ug/ml
18) T	n-Dotriacontane (C32)	18.851	146309	0.967 ug/ml
19) T	n-Tetratriacontane (C34)	19.603	259536	1.698 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE083124AL\
Data File : FE049836.D
Signal(s) : FID1B.ch
Acq On : 30 Aug 2024 06:08
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Aug 31 04:12:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 081424.M
Quant Title : GC Extractables
QLast Update : Wed Aug 14 11:05:17 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

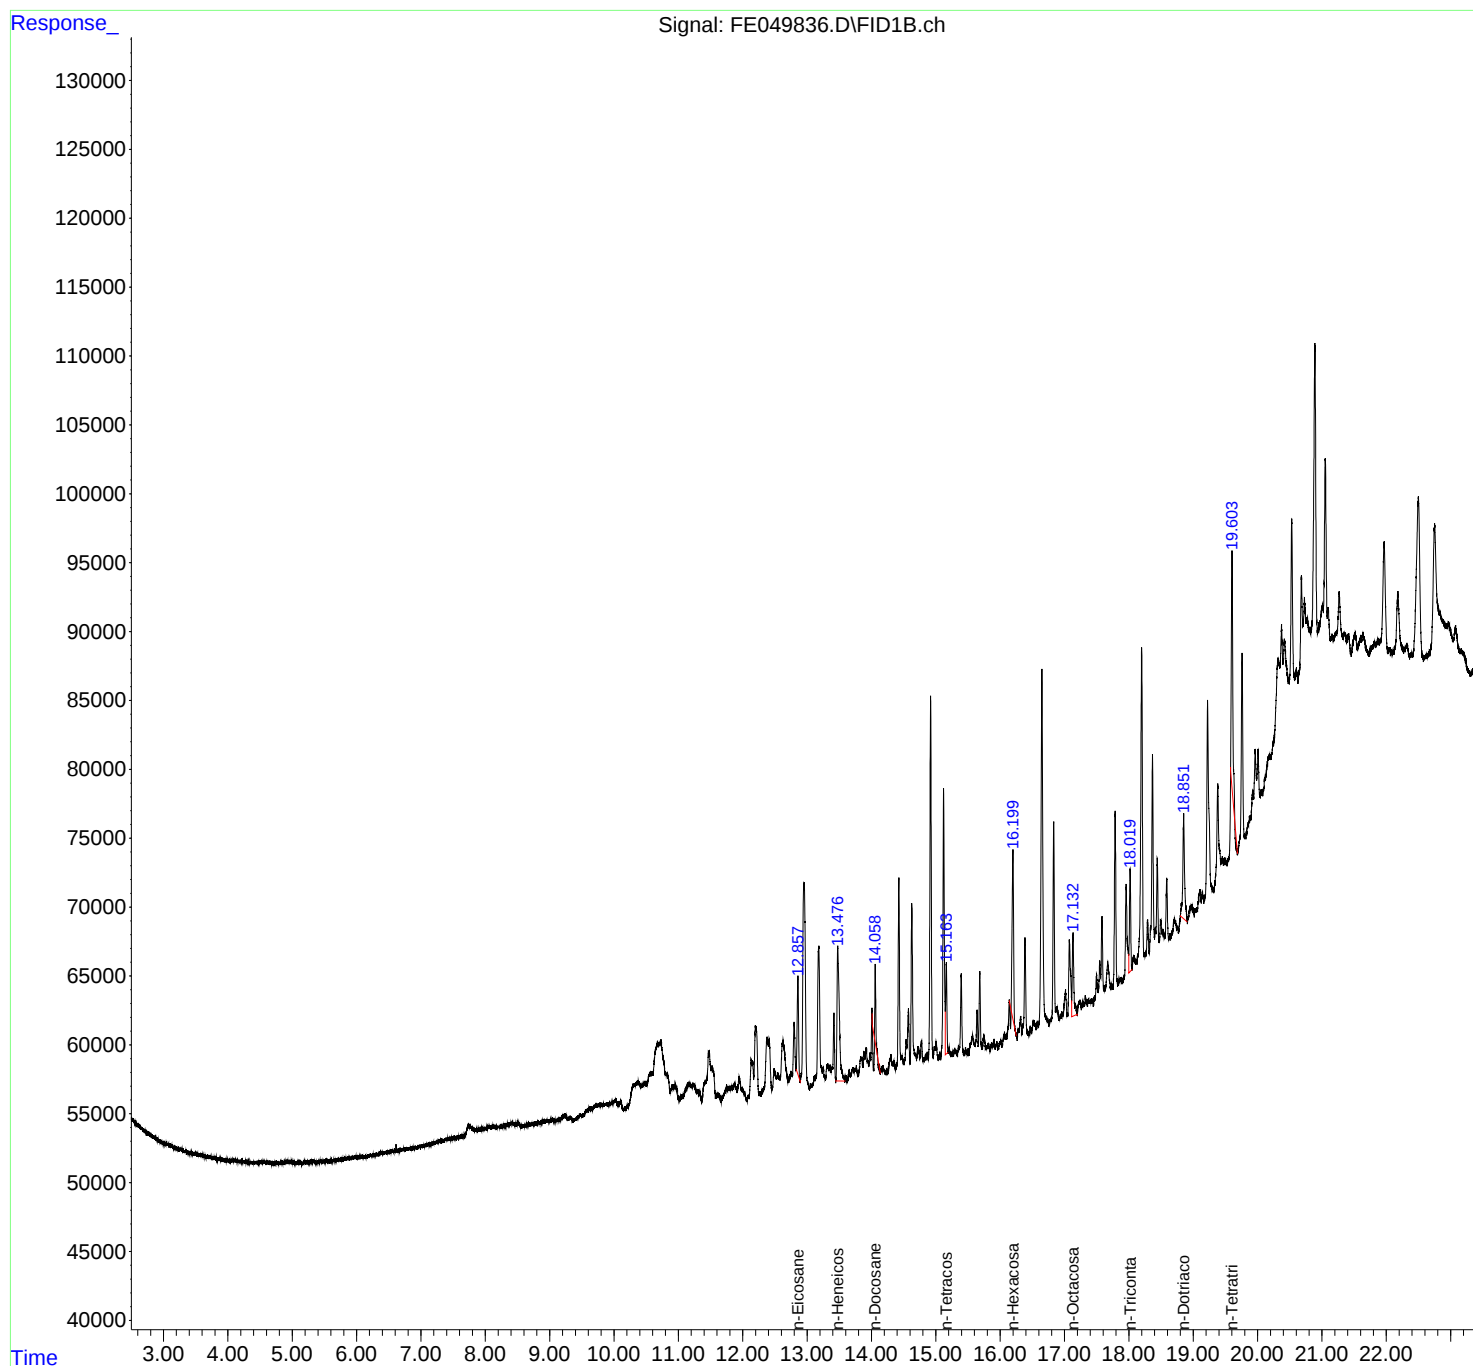


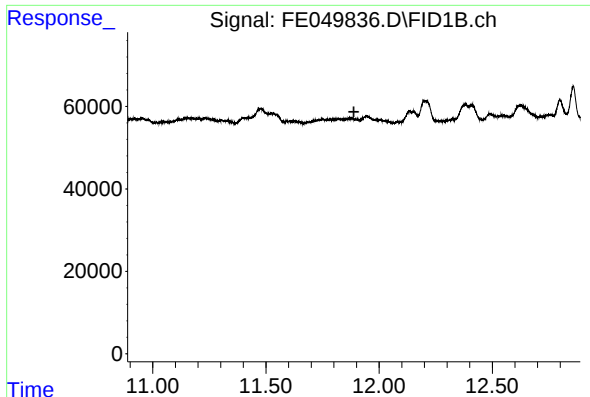

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.888 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
MECL2

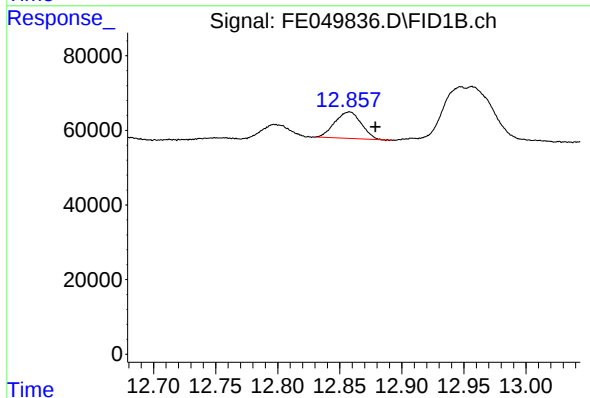


#10 n-Eicosane (C20)

R.T.: 12.857 min
Delta R.T.: -0.021 min
Response: 104858
Conc: 0.70 ug/ml

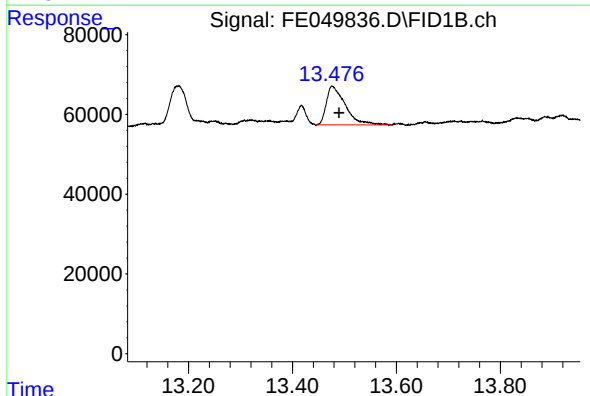


#11 n-Heneicosane (C21)

R.T.: 13.477 min
Delta R.T.: -0.013 min
Response: 245910
Conc: 1.68 ug/ml

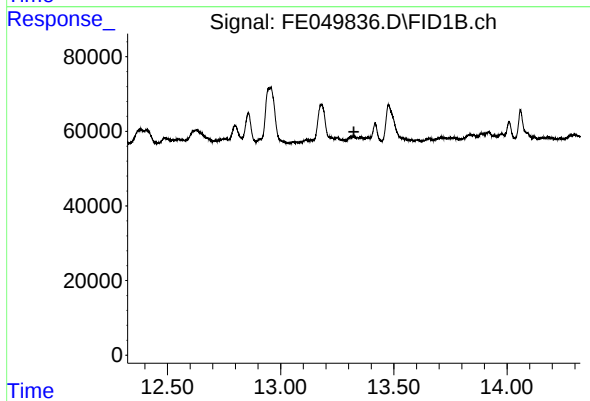

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.323 min
Response: 0
Conc: N.D.

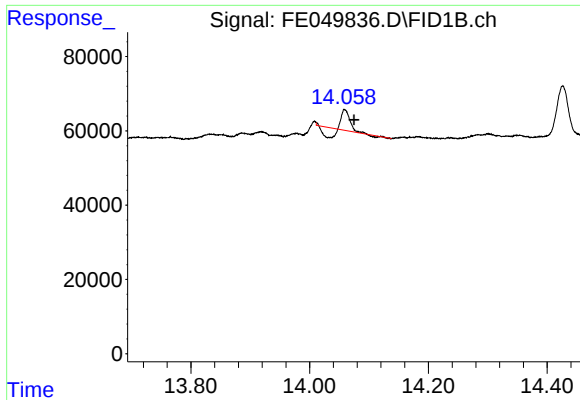

#13 n-Docosane (C22)


R.T.: 14.060 min
Delta R.T.: -0.016 min
Response: 27193
Conc: 0.19 ug/ml

Instrument :
FID_E
ClientSampleId :
MECL2

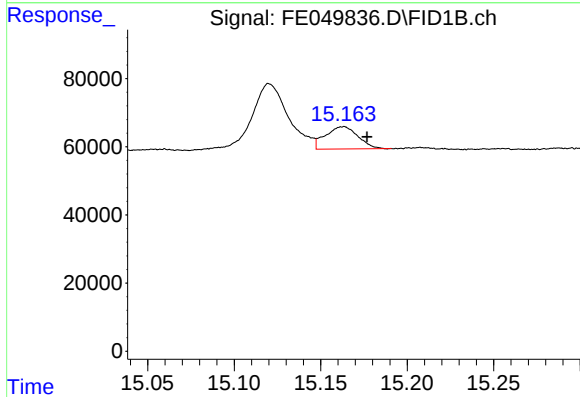


#14 n-Tetracosane (C24)

R.T.: 15.163 min
Delta R.T.: -0.014 min
Response: 86165
Conc: 0.59 ug/ml

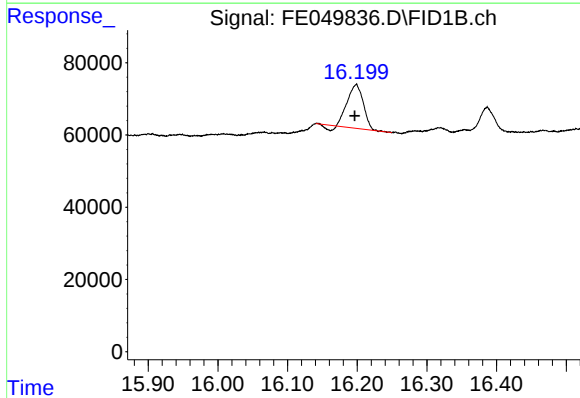


#15 n-Hexacosane (C26)

R.T.: 16.198 min
Delta R.T.: 0.002 min
Response: 179149
Conc: 1.24 ug/ml

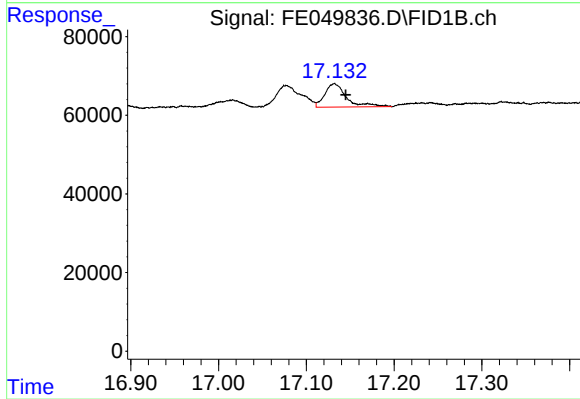

#16 n-Octacosane (C28)


R.T.: 17.132 min
Delta R.T.: -0.013 min
Response: 102277
Conc: 0.71 ug/ml

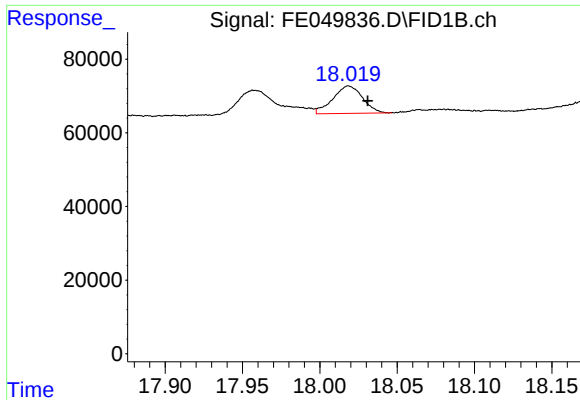

#17 n-Tricontane (C30)


R.T.: 18.019 min
Delta R.T.: -0.012 min
Response: 99194
Conc: 0.66 ug/ml

Instrument :
FID_E
ClientSampleId :
MECL2

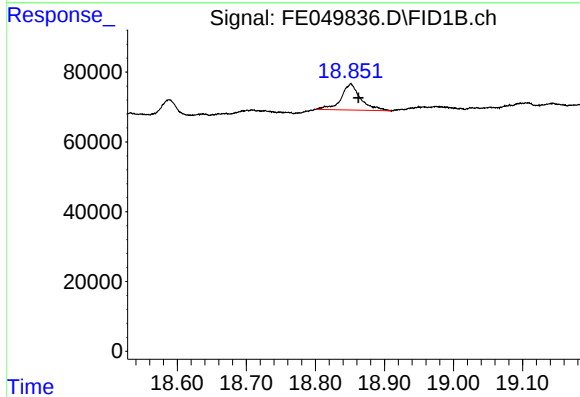

#18 n-Dotriacontane (C32)

R.T.: 18.851 min
Delta R.T.: -0.011 min
Response: 146309
Conc: 0.97 ug/ml

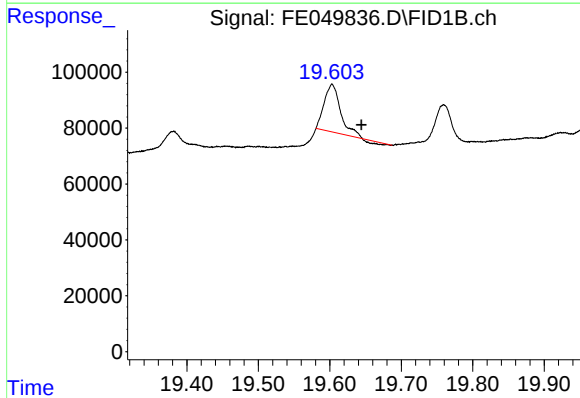

#19 n-Tetratriacontane (C34)

R.T.: 19.603 min
Delta R.T.: -0.041 min
Response: 259536
Conc: 1.70 ug/ml