

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090121\
 Data File : FE034278.D
 Signal(s) : FID1B.CH
 Acq On : 01 Sep 2021 11:38
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Sep 02 14:04:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE081621.M
 Quant Title :
 QLast Update : Mon Aug 16 16:04:52 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.413	5353238	15.507 ug/ml
12) N-OCTACOSANE	16.824	4997305	15.369 ug/ml
13) N-TRIACONTANE	17.708	337928	1.097 ug/ml
14) N-DOTRIACONTANE	18.537	479455	1.647 ug/ml
15) N-TETRATRIACONTANE	19.320	417636	1.666 ug/ml
16) N-HEXATRIACONTANE	20.060	293841	1.279 ug/ml
17) N-OCTATRIACONTANE	20.787	369617	1.829 ug/ml
18) N-TETRACONTANE	21.682	466236	2.713 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090121\
Data File : FE034278.D
Signal(s) : FID1B.CH
Acq On : 01 Sep 2021 11:38
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Sep 02 14:04:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE081621.M
Quant Title :
QLast Update : Mon Aug 16 16:04:52 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

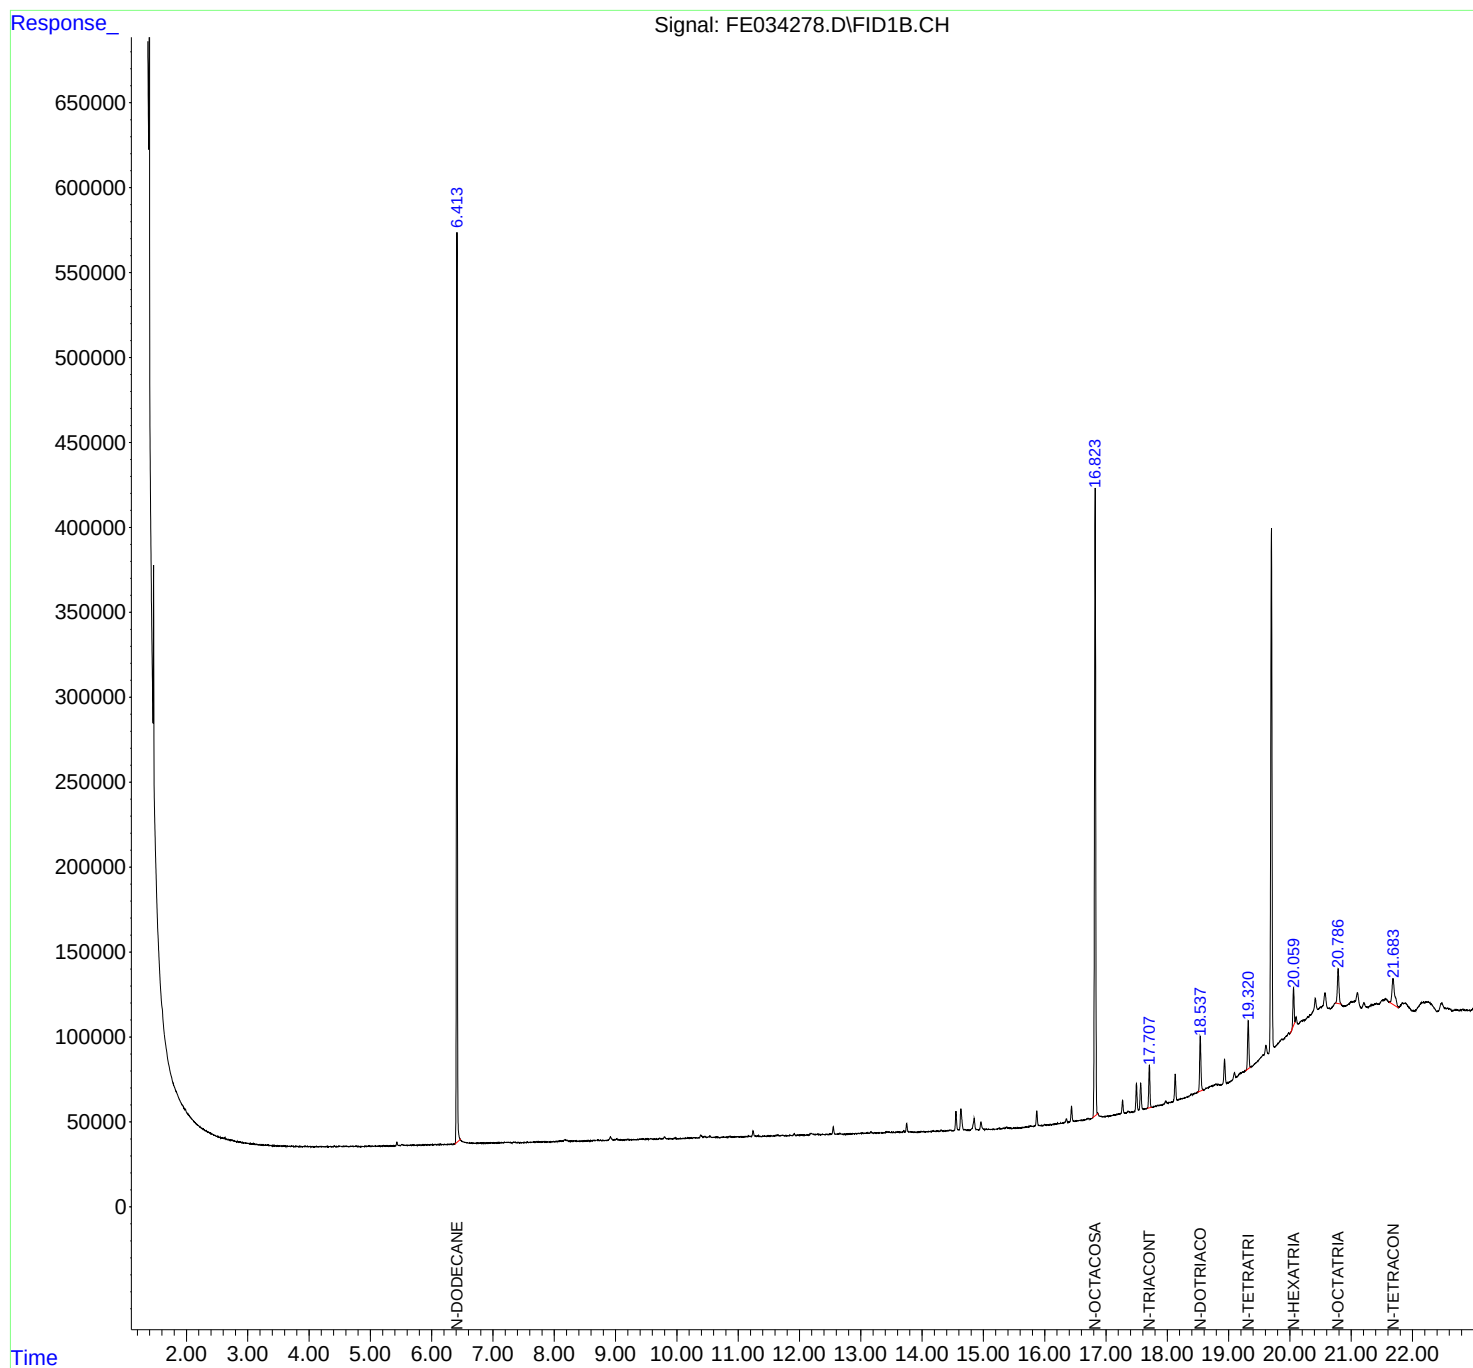


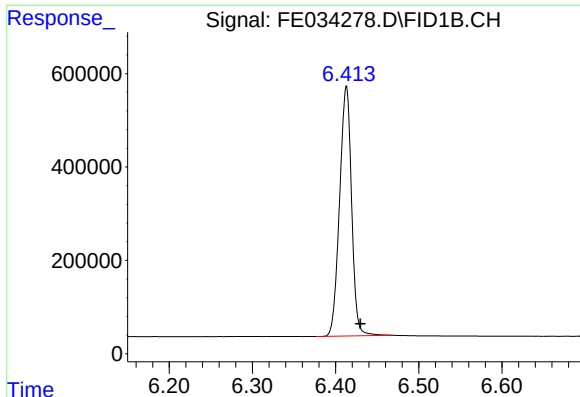

#3 N-DODECANE


R.T.: 6.413 min
Delta R.T.: -0.017 min
Response: 5353238
Conc: 15.51 ug/ml

Instrument :
FID_E
ClientSampleId :
RT MARKER

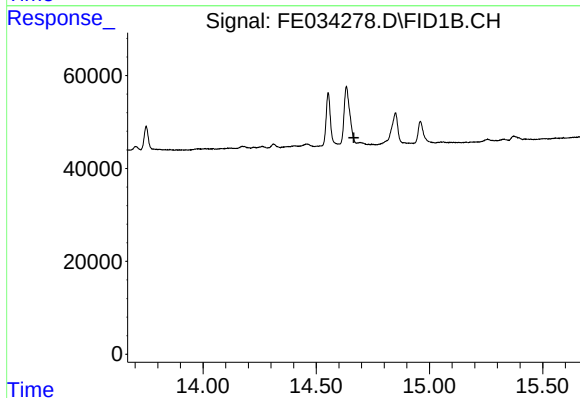


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.666 min
Response: 0
Conc: N.D.

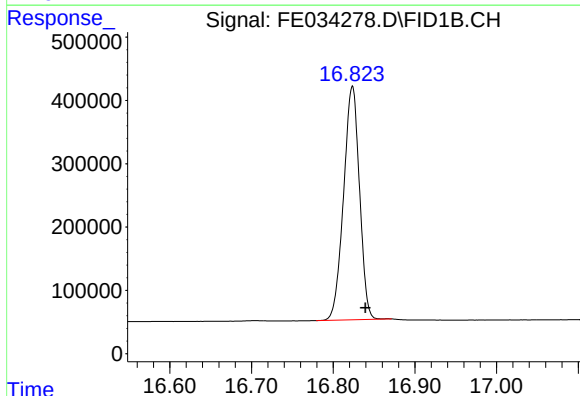


#12 N-OCTACOSANE

R.T.: 16.824 min
Delta R.T.: -0.016 min
Response: 4997305
Conc: 15.37 ug/ml

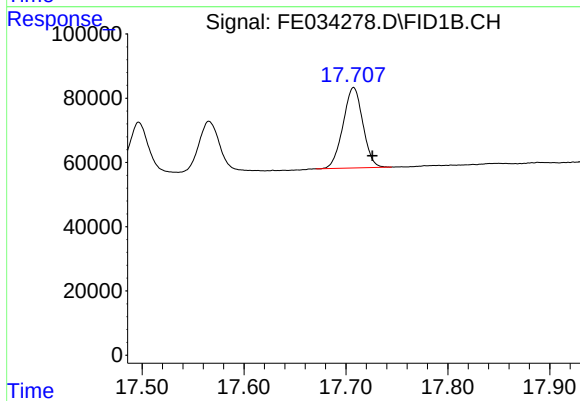

#13 N-TRIACONTANE


R.T.: 17.708 min
Delta R.T.: -0.018 min
Response: 337928
Conc: 1.10 ug/ml

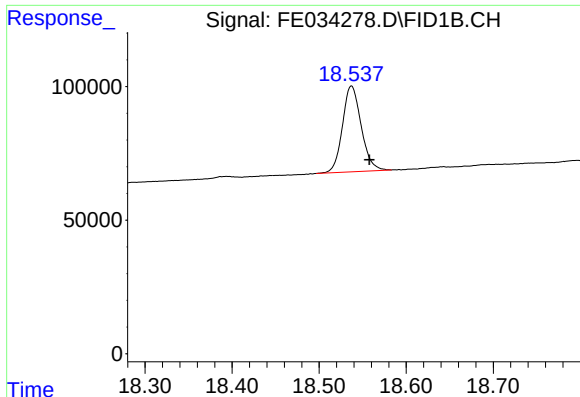

#14 N-DOTRIACONTANE


R.T.: 18.537 min
Delta R.T.: -0.021 min
Response: 479455
Conc: 1.65 ug/ml

Instrument :
FID_E
ClientSampleId :
RT MARKER

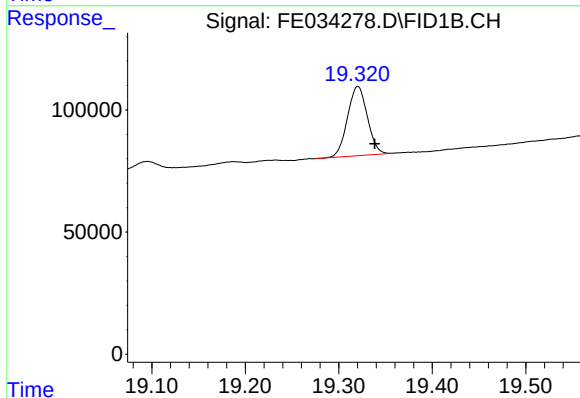


#15 N-TETRATRIACONTANE

R.T.: 19.320 min
Delta R.T.: -0.018 min
Response: 417636
Conc: 1.67 ug/ml

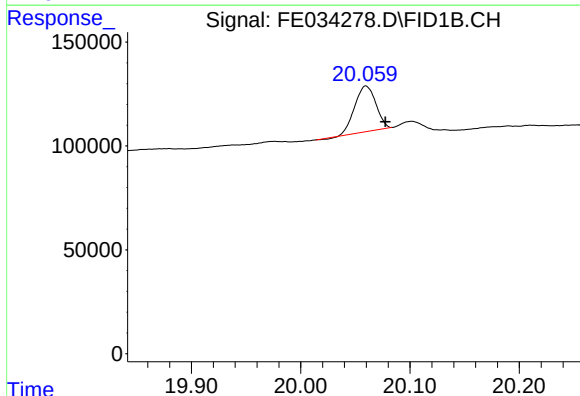


#16 N-HEXATRIACONTANE

R.T.: 20.060 min
Delta R.T.: -0.018 min
Response: 293841
Conc: 1.28 ug/ml

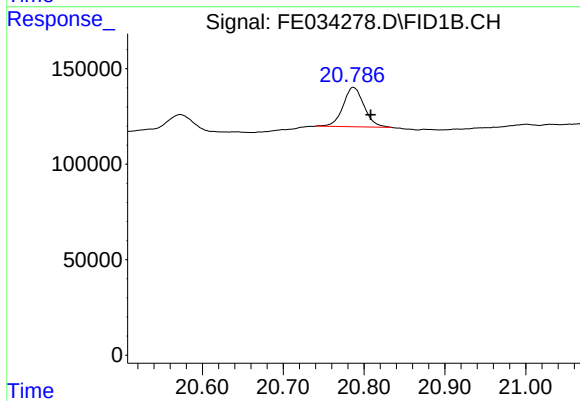

#17 N-OCTATRIACONTANE

R.T.: 20.787 min
Delta R.T.: -0.022 min
Response: 369617
Conc: 1.83 ug/ml

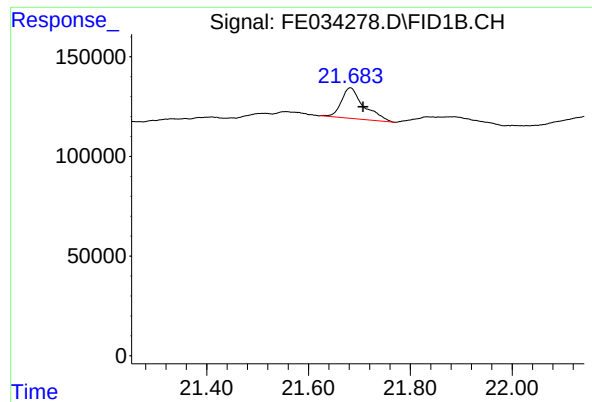

#18 N-TETRACONTANE

R.T.: 21.682 min
Delta R.T.: -0.025 min
Response: 466236
Conc: 2.71 ug/ml

Instrument :
FID_E
ClientSampleId :
RT MARKER