

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090123\
Data File : FE044081.D
Signal(s) : FID1B.ch
Acq On : 01 Sep 2023 09:42
Operator : YP\AJ
Sample : PB154670BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 01 23:59:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE083023.M
Quant Title :
QLast Update : Thu Aug 31 02:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.022	3533244	24.100 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.083	52918	0.353 ug/ml
14) N-DOTRIACONTANE	18.918	69270	0.509 ug/ml
15) N-TETRATRIACONTANE	19.702	58646	0.487 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090123\
Data File : FE044081.D
Signal(s) : FID1B.ch
Acq On : 01 Sep 2023 09:42
Operator : YP\AJ
Sample : PB154670BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 01 23:59:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE083023.M
Quant Title :
QLast Update : Thu Aug 31 02:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

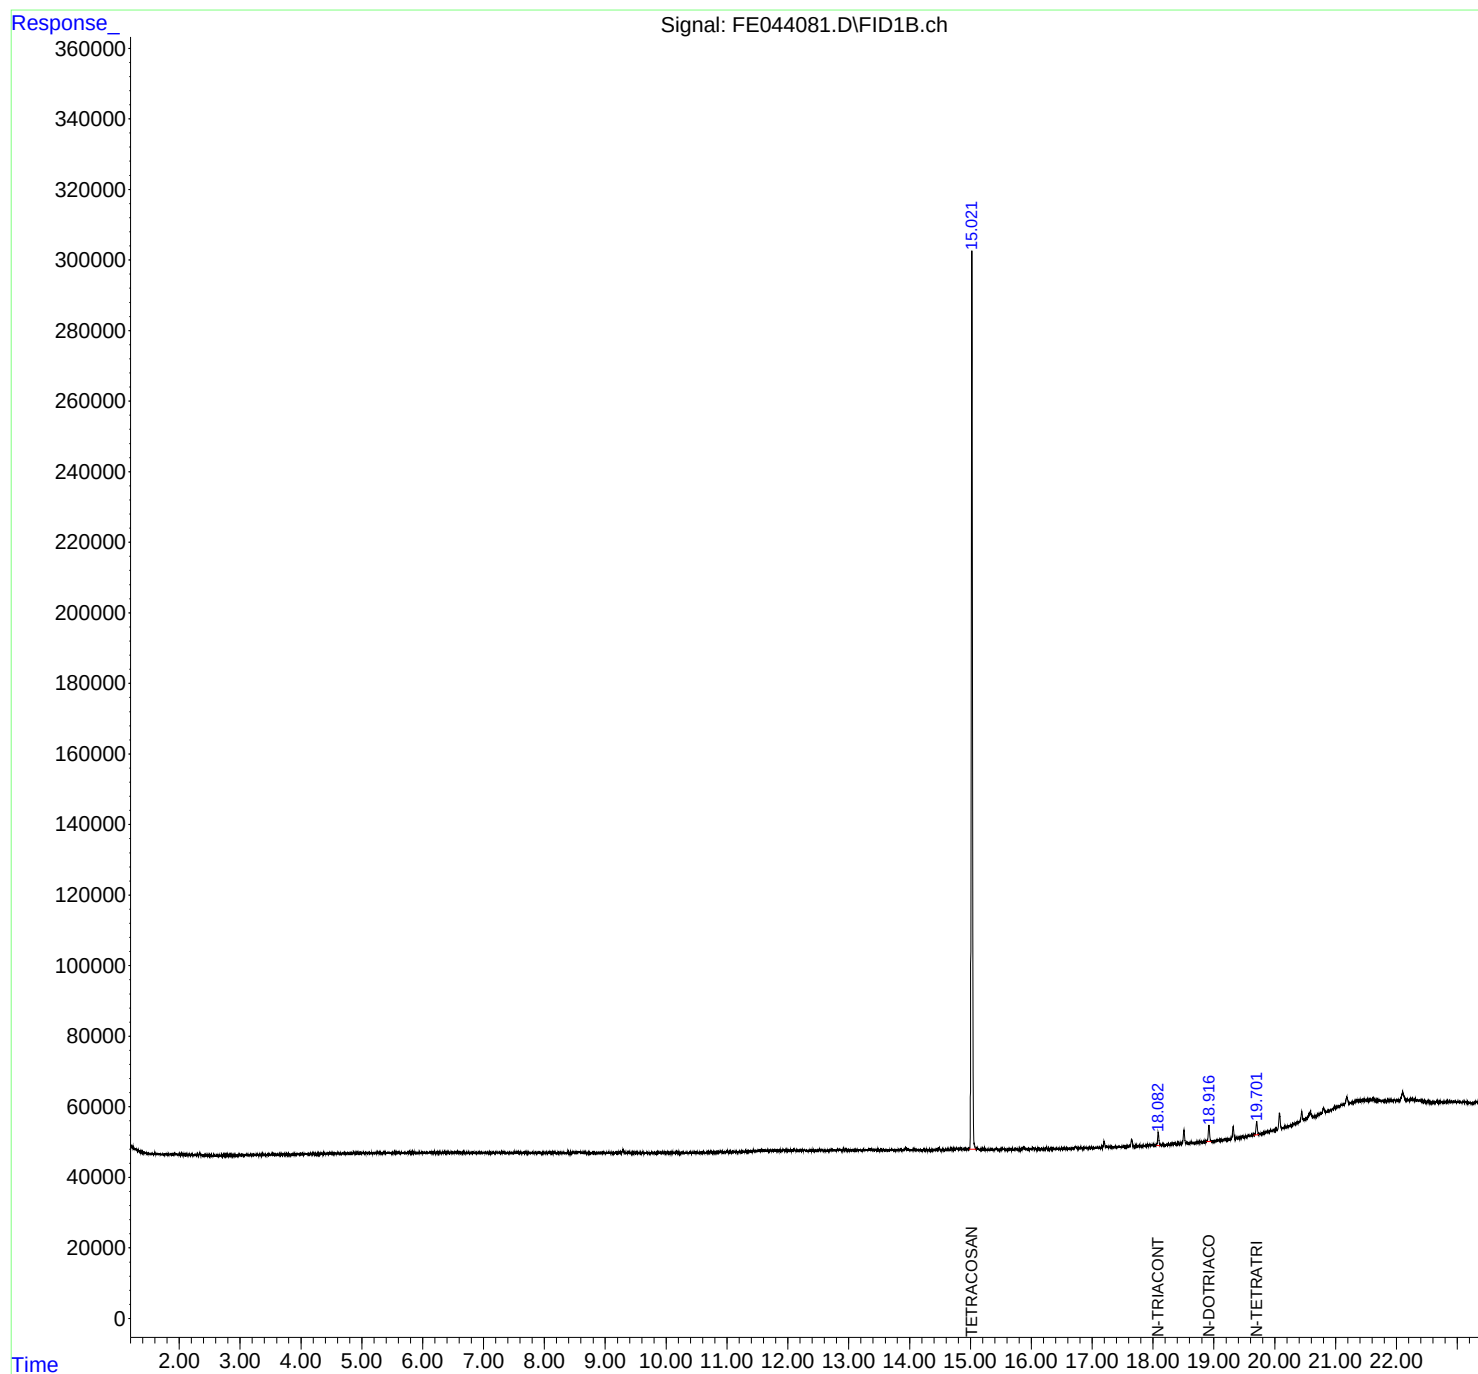


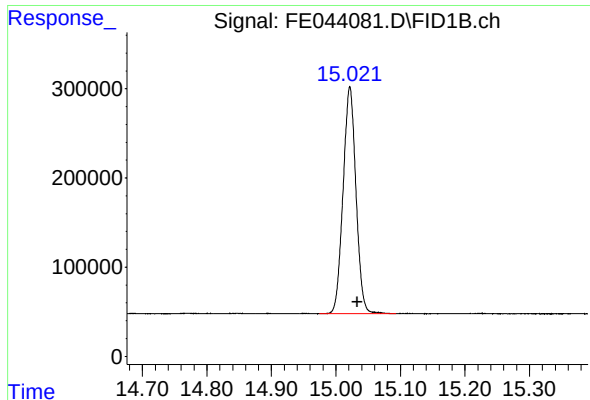

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.022 min
Delta R.T.: -0.012 min
Response: 3533244
Conc: 24.10 ug/ml

Instrument :
FID_E
ClientSampleId :

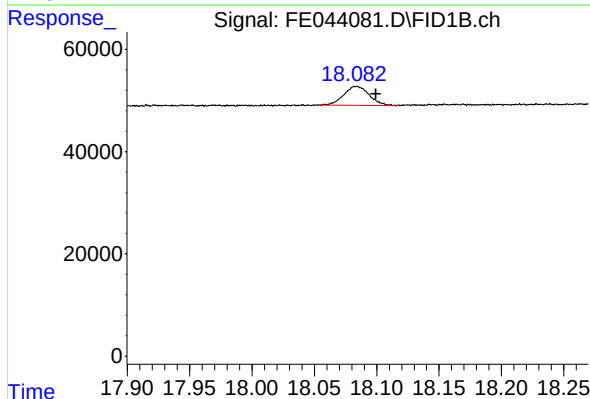


#13 N-TRIACONTANE

R.T.: 18.083 min
Delta R.T.: -0.016 min
Response: 52918
Conc: 0.35 ug/ml

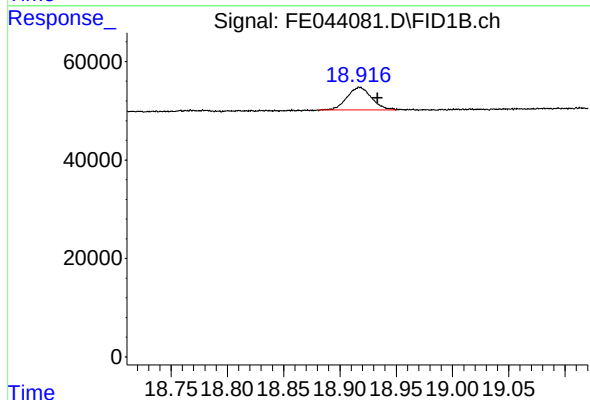

#14 N-DOTRIACONTANE

R.T.: 18.918 min
Delta R.T.: -0.016 min
Response: 69270
Conc: 0.51 ug/ml

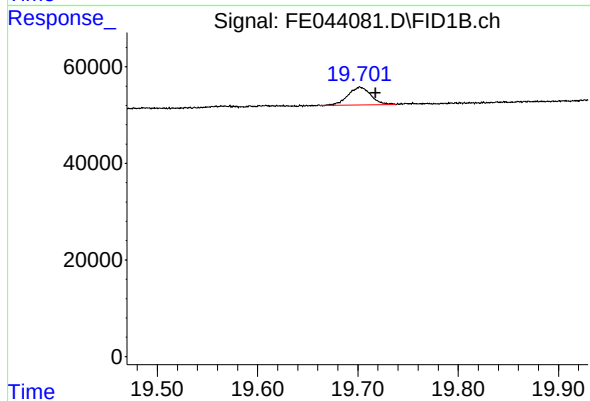

#15 N-TETRATRIACONTANE

R.T.: 19.702 min
Delta R.T.: -0.016 min
Response: 58646
Conc: 0.49 ug/ml