

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090123\
 Data File : FE044089.D
 Signal(s) : FID1B.ch
 Acq On : 01 Sep 2023 14:14
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Sep 02 00:00:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE083023.M
 Quant Title :
 QLast Update : Thu Aug 31 02:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.735	3183212	18.687 ug/ml
12) N-OCTACOSANE	17.195	2748170	17.579 ug/ml
17) N-OCTATRIACONTANE	21.180	90199	0.904 ug/ml
18) N-TETRACONTANE	22.097	216449	2.257 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE090123\
Data File : FE044089.D
Signal(s) : FID1B.ch
Acq On : 01 Sep 2023 14:14
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Sep 02 00:00:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE083023.M
Quant Title :
QLast Update : Thu Aug 31 02:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

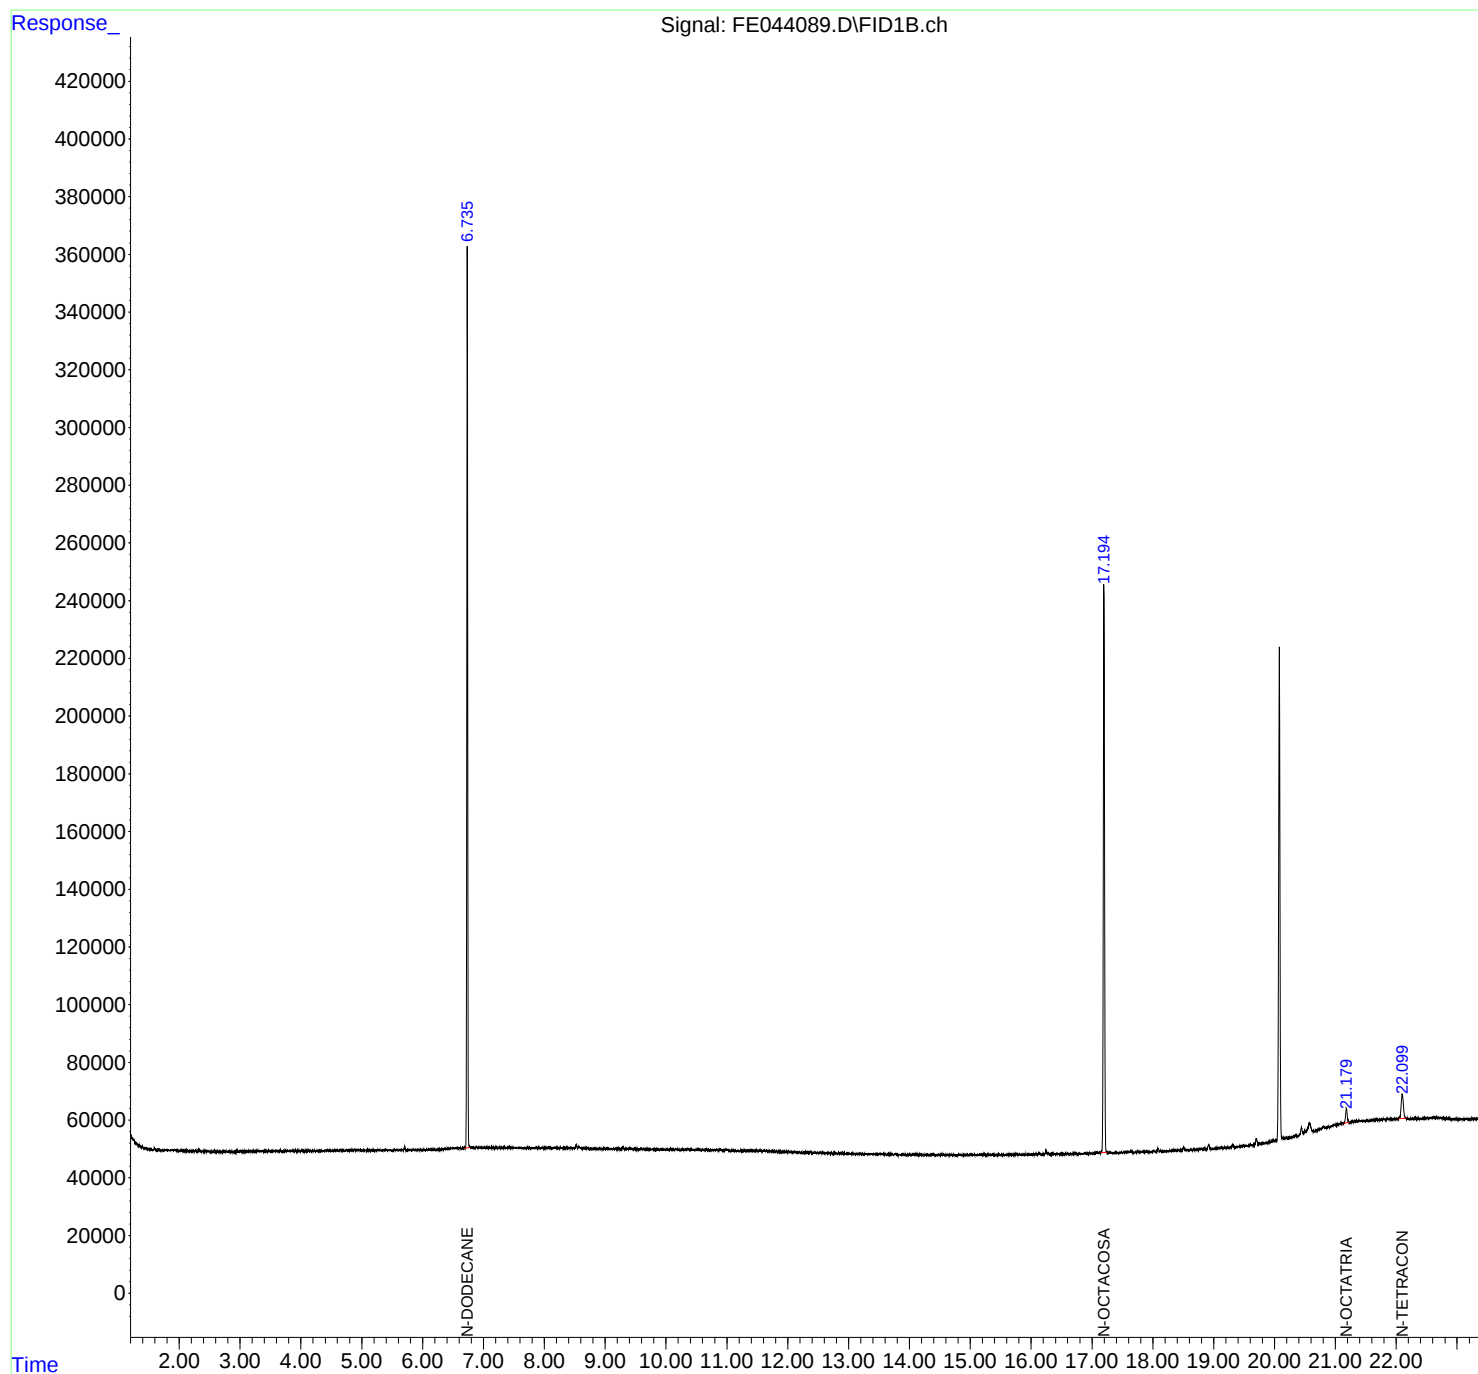


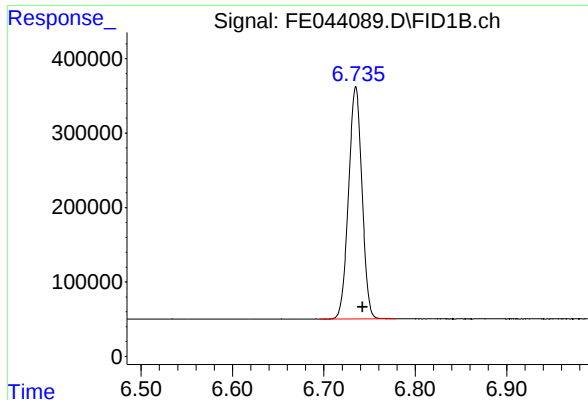

#3 N-DODECANE


R.T.: 6.735 min
Delta R.T.: -0.007 min
Response: 3183212
Conc: 18.69 ug/ml

Instrument :
FID_E
ClientSampleId :

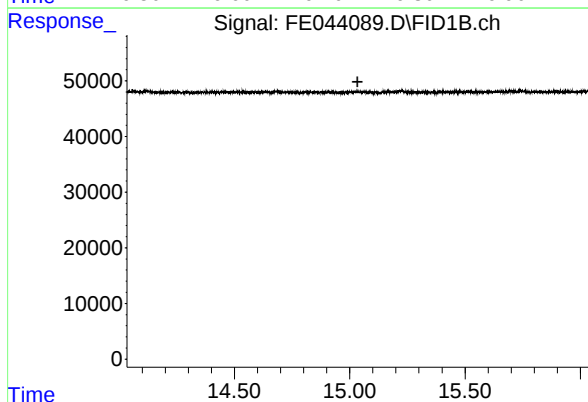


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 15.034 min
Response: 0
Conc: N.D.

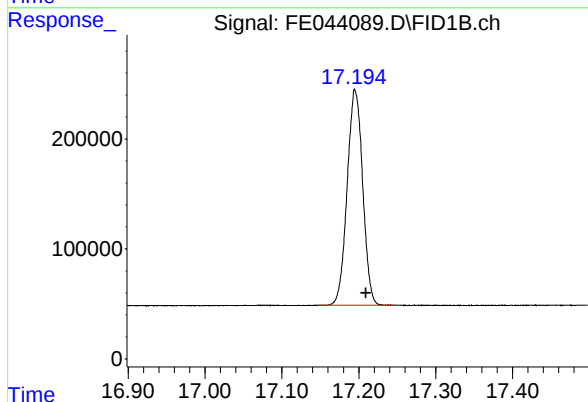


#12 N-OCTACOSANE

R.T.: 17.195 min
Delta R.T.: -0.014 min
Response: 2748170
Conc: 17.58 ug/ml

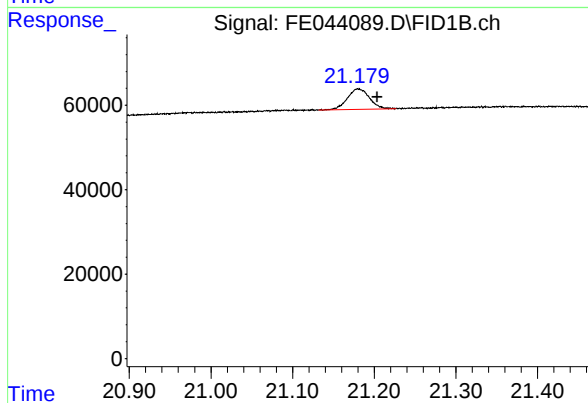

#17 N-OCTATRIACONTANE

R.T.: 21.180 min
Delta R.T.: -0.024 min
Response: 90199
Conc: 0.90 ug/ml

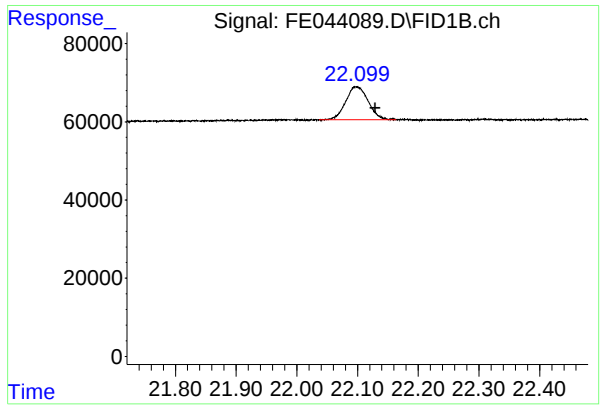

#18 N-TETRACONTANE

R.T.: 22.097 min
Delta R.T.: -0.033 min
Response: 216449
Conc: 2.26 ug/ml

Instrument :
FID_E
ClientSampleId :